

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019668.D
 Acq On : 16 Dec 2020 12:36
 Operator : SY/MD
 Sample : VV1216WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	378489	369158	15.45%	1.972%
2	1.569	142	149	163	rVB	286621	321978	13.47%	1.720%
3	2.110	307	317	347	rVB	583855	898638	37.60%	4.800%
4	2.817	535	537	542	rBV2	730	452	0.02%	0.002%
5	2.907	561	565	571	rVB3	642	757	0.03%	0.004%
6	2.936	571	574	576	rBV2	489	391	0.02%	0.002%
7	3.023	596	601	602	rBV2	544	483	0.02%	0.003%
8	3.061	611	613	616	rBV3	518	419	0.02%	0.002%
9	3.106	621	627	628	rBV2	538	463	0.02%	0.002%
10	3.315	688	692	693	rBV2	361	286	0.01%	0.002%
11	3.364	705	707	711	rBV2	536	410	0.02%	0.002%
12	3.505	748	751	757	rVB3	370	328	0.01%	0.002%
13	3.537	759	761	764	rBV	447	241	0.01%	0.001%
14	3.576	769	773	776	rBV2	385	338	0.01%	0.002%
15	3.650	794	796	800	rVB3	574	310	0.01%	0.002%
16	3.727	817	820	823	rVB2	307	218	0.01%	0.001%
17	3.749	824	827	830	rBV2	362	285	0.01%	0.002%
18	3.788	833	839	841	rBV3	360	408	0.02%	0.002%
19	3.830	850	852	856	rVB3	425	299	0.01%	0.002%
20	3.884	856	869	905	rBV	170476	519385	21.73%	2.774%
21	4.351	997	1014	1040	rBV	378207	930400	38.93%	4.970%
22	4.614	1092	1096	1100	rBV3	917	938	0.04%	0.005%
23	4.724	1128	1130	1132	rBV	466	224	0.01%	0.001%
24	4.762	1140	1142	1144	rBV	460	218	0.01%	0.001%
25	4.894	1179	1183	1185	rBV3	371	301	0.01%	0.002%
26	5.048	1212	1231	1263	rVV2	918218	2389827	100.00%	12.765%
27	5.325	1313	1317	1318	rBV3	811	510	0.02%	0.003%
28	5.454	1354	1357	1360	rBV3	792	656	0.03%	0.004%
29	5.537	1378	1383	1386	rBV5	782	772	0.03%	0.004%
30	5.618	1392	1408	1441	rBV	790611	1580047	66.12%	8.440%
31	5.910	1487	1499	1512	rBV3	13650	29668	1.24%	0.158%
32	5.978	1518	1520	1521	rBV2	444	232	0.01%	0.001%
33	6.071	1532	1549	1580	rBV	526201	1082890	45.31%	5.784%
34	6.312	1621	1624	1625	rBV2	730	428	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019668.D
 Acq On : 16 Dec 2020 12:36
 Operator : SY/MD
 Sample : VV1216WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.399	1648	1651	1654	rBV2	822	500	0.02%	0.003%
36	6.489	1675	1679	1681	rBV3	570	395	0.02%	0.002%
37	6.547	1693	1697	1698	rBV	559	363	0.02%	0.002%
38	6.617	1712	1719	1721	rBV4	628	627	0.03%	0.003%
39	6.634	1722	1724	1725	rBV2	601	212	0.01%	0.001%
40	6.711	1746	1748	1755	rVB3	585	599	0.03%	0.003%
41	6.817	1779	1781	1784	rBV2	610	344	0.01%	0.002%
42	6.891	1801	1804	1807	rVV2	365	256	0.01%	0.001%
43	6.987	1820	1834	1860	rBV	315338	578658	24.21%	3.091%
44	7.318	1924	1937	1968	rBV	1089867	1899875	79.50%	10.148%
45	7.621	2021	2031	2058	rBV	220230	386357	16.17%	2.064%
46	7.907	2117	2120	2122	rBV2	815	571	0.02%	0.003%
47	8.090	2166	2177	2214	rBV	616105	1105506	46.26%	5.905%
48	8.502	2303	2305	2309	rBV3	573	431	0.02%	0.002%
49	8.685	2360	2362	2366	rVB2	848	517	0.02%	0.003%
50	8.704	2366	2368	2370	rBV2	602	349	0.01%	0.002%
51	8.752	2380	2383	2384	rBV	586	344	0.01%	0.002%
52	8.855	2403	2415	2438	rBV	1178571	1903592	79.65%	10.168%
53	9.129	2498	2500	2503	rBV3	535	284	0.01%	0.002%
54	9.286	2545	2549	2554	rBV4	593	715	0.03%	0.004%
55	9.376	2574	2577	2579	rBV2	409	258	0.01%	0.001%
56	9.399	2582	2584	2587	rVB	687	385	0.02%	0.002%
57	9.421	2587	2591	2594	rVB2	411	291	0.01%	0.002%
58	9.444	2594	2598	2602	rBV3	344	388	0.02%	0.002%
59	9.463	2602	2604	2606	rVB	474	240	0.01%	0.001%
60	9.479	2606	2609	2612	rBV	424	271	0.01%	0.001%
61	9.508	2614	2618	2621	rBV2	489	437	0.02%	0.002%
62	9.585	2638	2642	2646	rBV4	740	890	0.04%	0.005%
63	9.666	2665	2667	2670	rBV2	462	290	0.01%	0.002%
64	9.682	2670	2672	2675	rVV	371	218	0.01%	0.001%
65	9.810	2710	2712	2716	rVB2	857	502	0.02%	0.003%
66	9.839	2719	2721	2724	rVB3	595	307	0.01%	0.002%
67	9.855	2724	2726	2728	rBV	333	207	0.01%	0.001%
68	9.891	2736	2737	2743	rVB	417	211	0.01%	0.001%
69	9.990	2764	2768	2769	rBV2	510	364	0.02%	0.002%
70	10.219	2828	2839	2864	rVB	661069	1036772	43.38%	5.538%
71	10.395	2892	2894	2896	rVB2	615	216	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019668.D
 Acq On : 16 Dec 2020 12:36
 Operator : SY/MD
 Sample : VV1216WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.453	2908	2912	2914	rBV4	654	484	0.02%	0.003%
73	10.502	2924	2927	2931	rVB4	1043	708	0.03%	0.004%
74	10.527	2933	2935	2936	rVV	546	250	0.01%	0.001%
75	10.550	2940	2942	2945	rVB	710	373	0.02%	0.002%
76	10.617	2959	2963	2966	rBV3	671	605	0.03%	0.003%
77	10.666	2975	2978	2980	rBV2	544	364	0.02%	0.002%
78	10.810	3020	3023	3030	rVB5	915	721	0.03%	0.004%
79	10.855	3030	3037	3038	rBV4	813	712	0.03%	0.004%
80	10.926	3054	3059	3064	rBV3	824	830	0.03%	0.004%
81	11.042	3093	3095	3101	rVB3	571	428	0.02%	0.002%
82	11.080	3101	3107	3109	rBV2	525	538	0.02%	0.003%
83	11.154	3123	3130	3131	rBV4	629	566	0.02%	0.003%
84	11.196	3137	3143	3149	rVB6	1476	2076	0.09%	0.011%
85	11.254	3149	3161	3188	rBV	1249850	1934470	80.95%	10.333%
86	11.514	3239	3242	3244	rBV2	620	400	0.02%	0.002%
87	11.540	3248	3250	3251	rBV2	482	223	0.01%	0.001%
88	11.630	3265	3278	3297	rBV	1095660	1715169	71.77%	9.161%
89	11.874	3351	3354	3359	rBV4	616	558	0.02%	0.003%
90	12.119	3427	3430	3432	rBV	514	209	0.01%	0.001%
91	12.222	3458	3462	3465	rBV3	574	551	0.02%	0.003%
92	12.296	3483	3485	3487	rBV3	488	221	0.01%	0.001%
93	12.653	3593	3596	3606	rVB5	1363	1684	0.07%	0.009%
94	13.038	3712	3716	3720	rBV3	662	638	0.03%	0.003%
95	13.183	3759	3761	3765	rBV4	430	287	0.01%	0.002%
96	13.209	3765	3769	3773	rBV2	451	418	0.02%	0.002%
97	13.273	3785	3789	3797	rBV4	1952	2246	0.09%	0.012%
98	13.469	3848	3850	3852	rBV3	607	293	0.01%	0.002%
99	13.569	3879	3881	3886	rBV3	715	431	0.02%	0.002%
100	13.778	3944	3946	3949	rBV3	589	256	0.01%	0.001%


Sum of corrected areas: 18721809

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121620\
Data File : VV019668.D
Acq On : 16 Dec 2020 12:36
Operator : SY/MD
Sample : VV1216WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

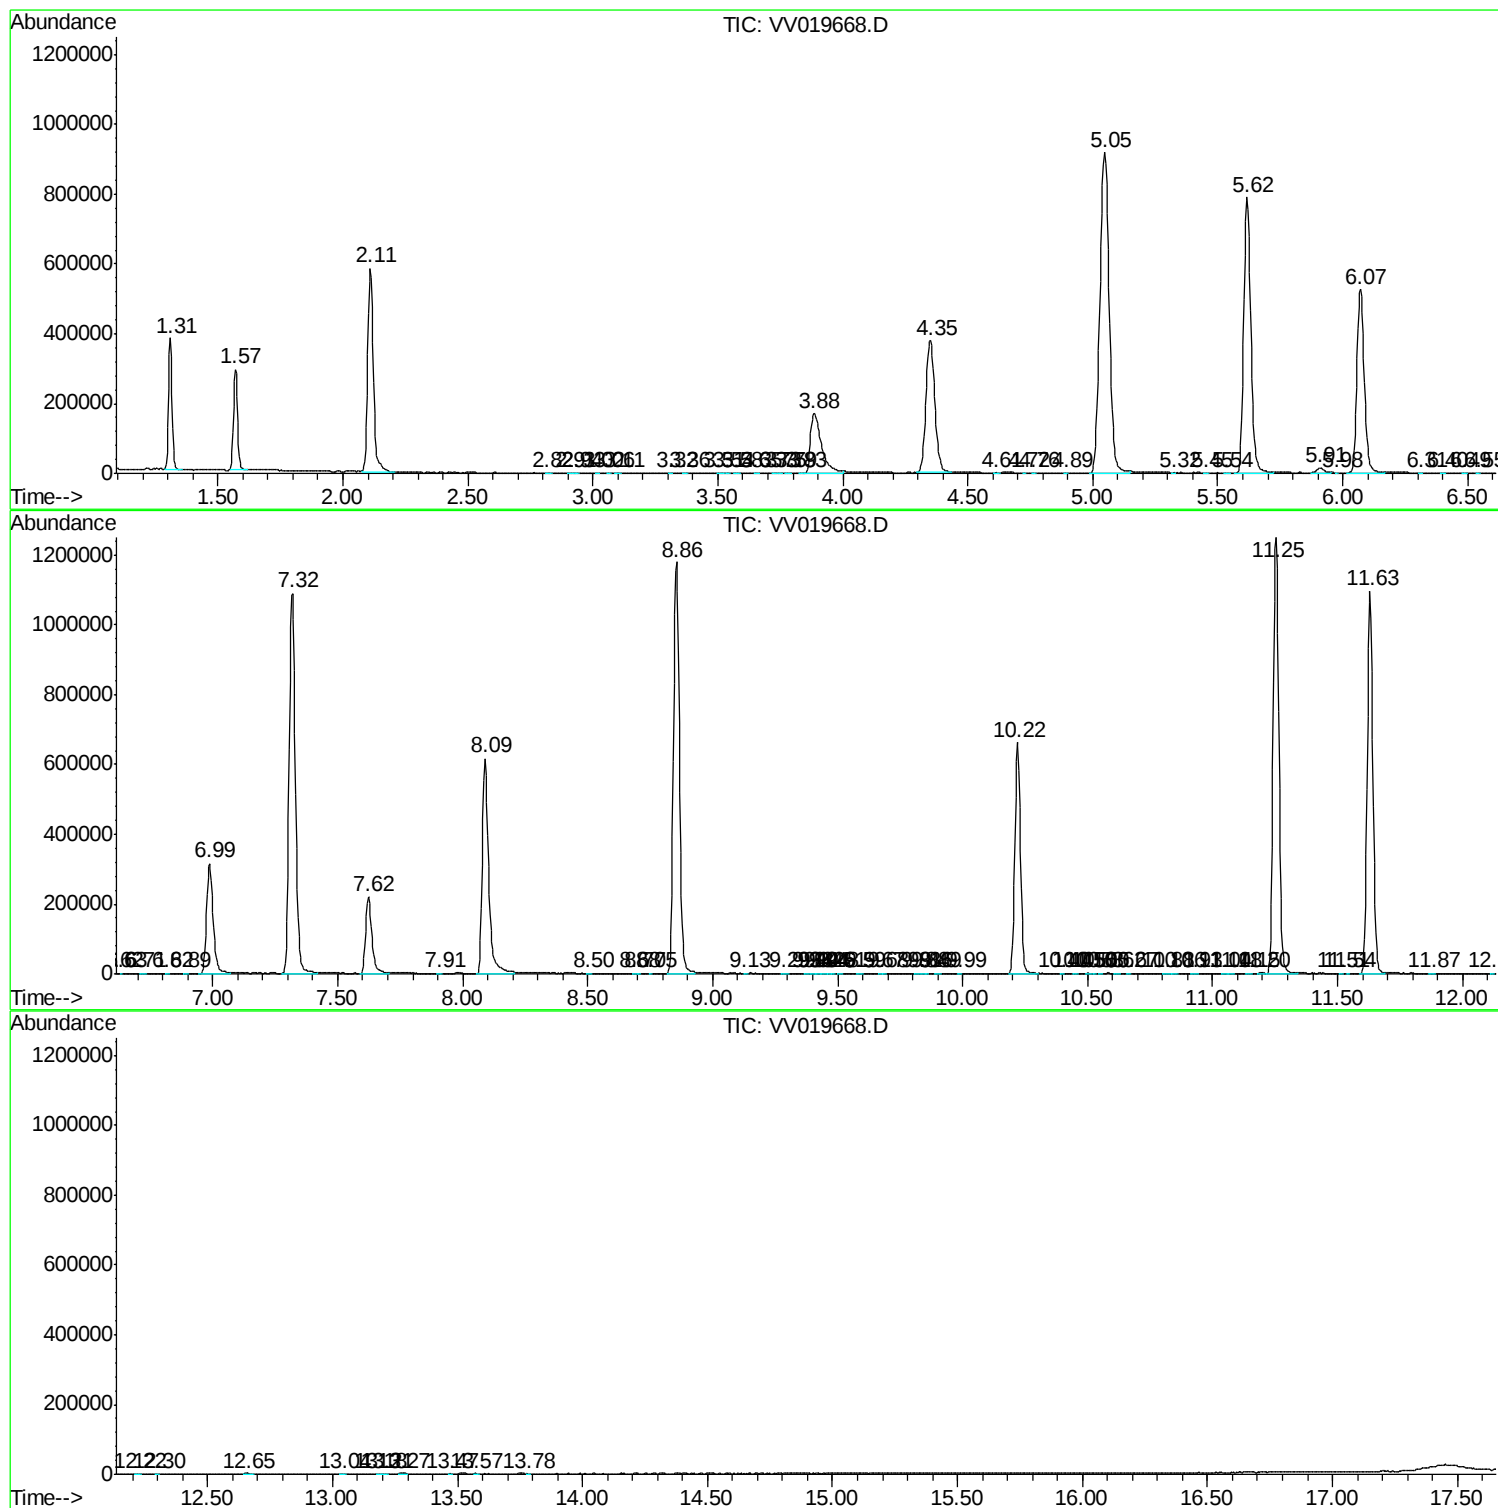

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121620\
Data File : VV019668.D
Acq On : 16 Dec 2020 12:36
Operator : SY/MD
Sample : VV1216WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121620\
Data File : VV019668.D
Acq On : 16 Dec 2020 12:36
Operator : SY/MD
Sample : VV1216WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc