

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019670.D
 Acq On : 16 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	335732	327869	14.54%	1.839%
2	1.573	142	150	163	rBV	261008	297107	13.18%	1.666%
3	2.113	308	318	334	rBV	524057	790748	35.08%	4.435%
4	2.833	539	542	546	rBV3	520	439	0.02%	0.002%
5	2.933	569	573	574	rBV	402	334	0.01%	0.002%
6	3.055	609	611	613	rVB3	480	213	0.01%	0.001%
7	3.151	639	641	643	rBV	343	189	0.01%	0.001%
8	3.168	643	646	649	rVV3	346	260	0.01%	0.001%
9	3.196	652	655	657	rBV	507	291	0.01%	0.002%
10	3.222	660	663	664	rBV	391	218	0.01%	0.001%
11	3.274	677	679	682	rVB2	491	212	0.01%	0.001%
12	3.290	682	684	689	rVB3	541	243	0.01%	0.001%
13	3.315	690	692	698	rBV3	275	265	0.01%	0.001%
14	3.344	698	701	704	rBV2	457	294	0.01%	0.002%
15	3.360	704	706	708	rVB2	249	87	0.00%	0.000%
16	3.380	708	712	714	rBV4	515	387	0.02%	0.002%
17	3.624	784	788	791	rBV3	701	562	0.02%	0.003%
18	3.778	832	836	837	rBV2	313	240	0.01%	0.001%
19	3.807	843	845	850	rBV3	403	389	0.02%	0.002%
20	3.891	856	871	925	rBV	169605	554501	24.60%	3.110%
21	4.354	999	1015	1047	rBV	359160	886623	39.33%	4.973%
22	4.666	1110	1112	1115	rBV3	476	337	0.01%	0.002%
23	4.714	1123	1127	1128	rBV3	741	387	0.02%	0.002%
24	4.791	1148	1151	1161	rBV4	499	816	0.04%	0.005%
25	4.839	1165	1166	1169	rBV2	537	273	0.01%	0.002%
26	4.974	1206	1208	1210	rBV2	278	149	0.01%	0.001%
27	5.052	1213	1232	1269	rBV2	876990	2254339	100.00%	12.645%
28	5.364	1327	1329	1330	rBV2	562	244	0.01%	0.001%
29	5.515	1373	1376	1378	rBV2	622	411	0.02%	0.002%
30	5.621	1396	1409	1438	rBV	783267	1556513	69.05%	8.730%
31	5.910	1487	1499	1519	rVB3	19339	45520	2.02%	0.255%
32	6.074	1535	1550	1583	rBV	498094	1023569	45.40%	5.741%
33	6.370	1640	1642	1645	rBV2	682	364	0.02%	0.002%
34	6.627	1719	1722	1726	rBV3	1167	1009	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019670.D
 Acq On : 16 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.714	1743	1749	1751	rBV4	676	599	0.03%	0.003%
36	6.801	1774	1776	1777	rBV4	273	131	0.01%	0.001%
37	6.810	1777	1779	1781	rVV	333	157	0.01%	0.001%
38	6.868	1793	1797	1800	rBV2	709	661	0.03%	0.004%
39	6.920	1808	1813	1815	rBV3	389	261	0.01%	0.001%
40	6.936	1815	1818	1820	rBV	453	245	0.01%	0.001%
41	6.990	1822	1835	1866	rBV	295823	542932	24.08%	3.045%
42	7.318	1924	1937	1955	rBV	1034093	1776746	78.81%	9.966%
43	7.624	2022	2032	2060	rBV	206191	362037	16.06%	2.031%
44	7.862	2103	2106	2107	rBV2	608	325	0.01%	0.002%
45	8.042	2156	2162	2167	rBV4	3843	5040	0.22%	0.028%
46	8.090	2167	2177	2212	rVV	598203	1073655	47.63%	6.022%
47	8.646	2347	2350	2353	rVB2	559	376	0.02%	0.002%
48	8.730	2373	2376	2379	rBV4	728	373	0.02%	0.002%
49	8.769	2386	2388	2391	rBV3	480	324	0.01%	0.002%
50	8.855	2403	2415	2441	rBV	1161863	1882295	83.50%	10.558%
51	9.148	2499	2506	2514	rBV5	4754	6925	0.31%	0.039%
52	9.264	2540	2542	2546	rBV3	646	477	0.02%	0.003%
53	9.306	2552	2555	2557	rBV2	620	450	0.02%	0.003%
54	9.415	2587	2589	2591	rVB	312	106	0.00%	0.001%
55	9.466	2603	2605	2610	rVB4	614	445	0.02%	0.002%
56	9.495	2612	2614	2615	rBV	267	116	0.01%	0.001%
57	9.572	2624	2638	2651	rBV6	7375	17038	0.76%	0.096%
58	9.704	2677	2679	2681	rBV2	469	242	0.01%	0.001%
59	9.727	2681	2686	2691	rVV6	1149	1355	0.06%	0.008%
60	9.772	2697	2700	2707	rVB5	611	595	0.03%	0.003%
61	9.823	2707	2716	2728	rBV7	2743	5831	0.26%	0.033%
62	9.904	2738	2741	2745	rBV3	719	462	0.02%	0.003%
63	9.923	2745	2747	2751	rVB2	545	304	0.01%	0.002%
64	9.949	2751	2755	2757	rBV2	584	395	0.02%	0.002%
65	10.006	2769	2773	2774	rBV2	452	302	0.01%	0.002%
66	10.106	2802	2804	2805	rBV2	313	119	0.01%	0.001%
67	10.170	2822	2824	2826	rBV	426	230	0.01%	0.001%
68	10.222	2828	2840	2862	rVB	625094	966505	42.87%	5.421%
69	10.325	2870	2872	2874	rBV2	719	326	0.01%	0.002%
70	10.386	2885	2891	2900	rVB4	4134	6004	0.27%	0.034%
71	10.656	2970	2975	2977	rBV3	730	587	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019670.D
 Acq On : 16 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.704	2984	2990	2998	rBV5	1359	1912	0.08%	0.011%
73	10.775	3010	3012	3014	rBV3	470	205	0.01%	0.001%
74	10.939	3053	3063	3076	rBV8	4848	12292	0.55%	0.069%
75	11.254	3149	3161	3184	rBV	1167992	1803573	80.00%	10.116%
76	11.479	3228	3231	3233	rBV2	534	281	0.01%	0.002%
77	11.492	3233	3235	3241	rVB4	809	573	0.03%	0.003%
78	11.540	3241	3250	3262	rBV5	3941	8449	0.37%	0.047%
79	11.630	3266	3278	3298	rVV	1011463	1596799	70.83%	8.956%
80	11.875	3352	3354	3357	rBV3	618	363	0.02%	0.002%
81	12.444	3529	3531	3533	rBV2	551	203	0.01%	0.001%
82	12.469	3536	3539	3542	rBV2	922	561	0.02%	0.003%
83	13.080	3727	3729	3733	rBV3	651	397	0.02%	0.002%
84	13.463	3845	3848	3853	rBV3	605	640	0.03%	0.004%
85	13.592	3886	3888	3891	rBV2	670	421	0.02%	0.002%
86	13.656	3906	3908	3916	rVB3	899	805	0.04%	0.005%
87	13.855	3968	3970	3975	rBV2	441	295	0.01%	0.002%
88	13.878	3975	3977	3980	rBV	526	356	0.02%	0.002%


Sum of corrected areas: 17828498

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121620\
Data File : VV019670.D
Acq On : 16 Dec 2020 13:24
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

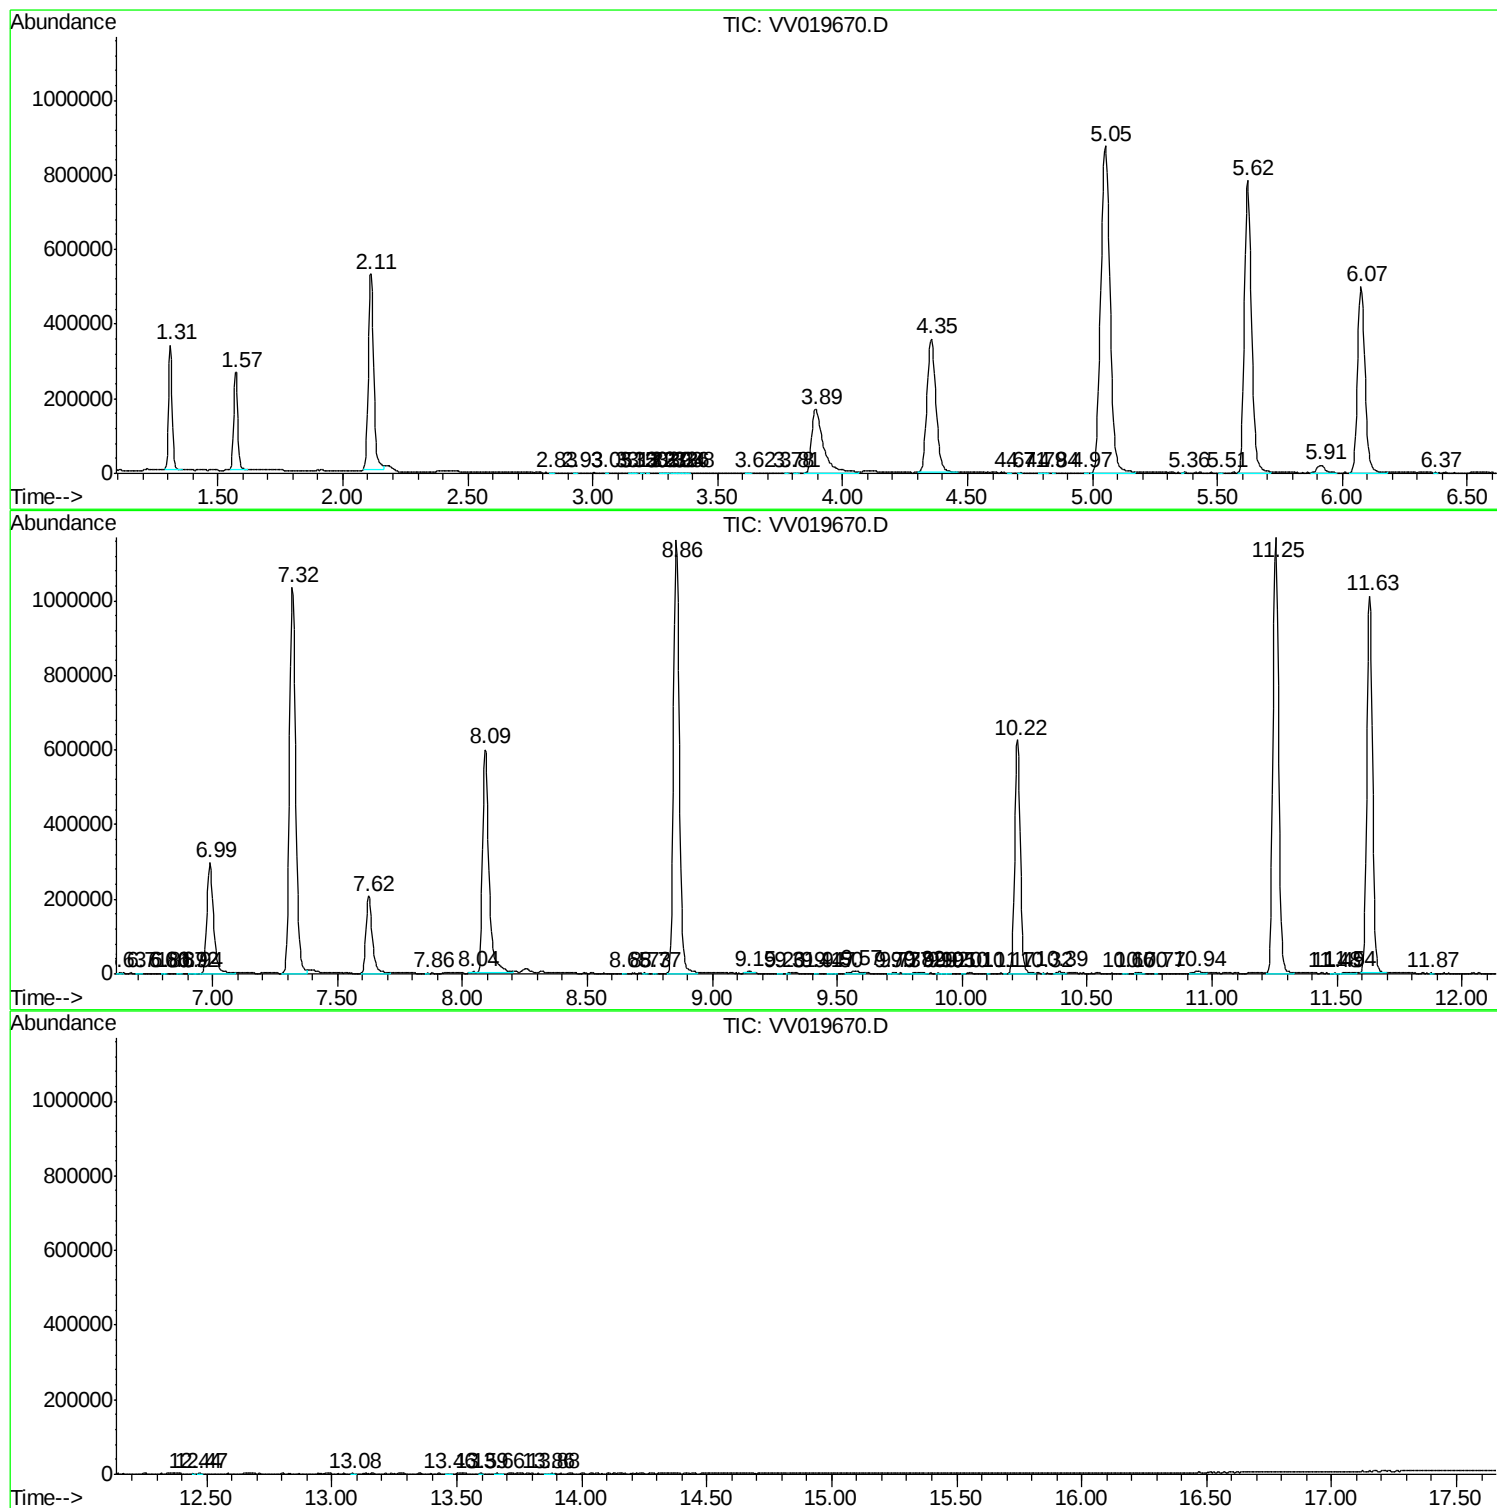

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121620\
Data File : VV019670.D
Acq On : 16 Dec 2020 13:24
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121620\
Data File : VV019670.D
Acq On : 16 Dec 2020 13:24
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc