

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019671.D
 Acq On : 16 Dec 2020 13:48
 Operator : SY/MD
 Sample : L5098-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	333720	335836	14.61%	1.933%
2	1.569	142	149	162	rBV	265473	302755	13.17%	1.743%
3	2.113	308	318	336	rBV	529946	804843	35.01%	4.632%
4	2.859	548	550	554	rBV3	433	323	0.01%	0.002%
5	2.910	565	566	569	rBV3	449	245	0.01%	0.001%
6	3.180	647	650	652	rBV3	460	342	0.01%	0.002%
7	3.354	698	704	709	rBV3	824	994	0.04%	0.006%
8	3.431	726	728	729	rBV	319	115	0.01%	0.001%
9	3.540	759	762	765	rBV2	441	353	0.02%	0.002%
10	3.582	772	775	778	rBV2	394	282	0.01%	0.002%
11	3.598	778	780	784	rVB2	323	263	0.01%	0.002%
12	3.627	784	789	790	rBV	322	247	0.01%	0.001%
13	3.675	800	804	807	rBV3	433	398	0.02%	0.002%
14	3.691	807	809	815	rBV3	371	246	0.01%	0.001%
15	3.765	818	832	852	rVB5	8341	22811	0.99%	0.131%
16	3.842	852	856	857	rBV	722	538	0.02%	0.003%
17	3.891	860	871	912	rBV	162986	487582	21.21%	2.806%
18	4.354	1000	1015	1041	rBV	363169	880495	38.30%	5.068%
19	4.894	1182	1183	1186	rVB	358	162	0.01%	0.001%
20	4.916	1186	1190	1192	rBV2	440	324	0.01%	0.002%
21	4.936	1194	1196	1198	rBV	604	292	0.01%	0.002%
22	5.051	1214	1232	1275	rBV2	898248	2299007	100.00%	13.233%
23	5.621	1396	1409	1441	rBV	709966	1419497	61.74%	8.170%
24	5.813	1467	1469	1476	rBV5	770	665	0.03%	0.004%
25	5.910	1488	1499	1519	rVB2	23058	49055	2.13%	0.282%
26	6.074	1536	1550	1582	rBV	507322	1036725	45.09%	5.967%
27	6.604	1714	1715	1716	rBV	424	129	0.01%	0.001%
28	6.614	1716	1718	1721	rVB2	592	296	0.01%	0.002%
29	6.640	1721	1726	1727	rBV2	741	595	0.03%	0.003%
30	6.717	1748	1750	1751	rBV	479	175	0.01%	0.001%
31	6.746	1757	1759	1763	rVB3	461	269	0.01%	0.002%
32	6.784	1767	1771	1773	rBV3	532	417	0.02%	0.002%
33	6.842	1786	1789	1792	rBV	247	201	0.01%	0.001%
34	6.929	1812	1816	1817	rBV2	385	273	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019671.D
 Acq On : 16 Dec 2020 13:48
 Operator : SY/MD
 Sample : L5098-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.990	1823	1835	1867	rBV	287965	522766	22.74%	3.009%
36	7.318	1925	1937	1972	rBV	1047369	1821491	79.23%	10.484%
37	7.624	2022	2032	2055	rBV	198926	347120	15.10%	1.998%
38	8.093	2167	2178	2216	rBV	593511	1100484	47.87%	6.334%
39	8.469	2293	2295	2297	rBV	375	245	0.01%	0.001%
40	8.791	2393	2395	2398	rBV3	477	204	0.01%	0.001%
41	8.855	2403	2415	2447	rBV	1070460	1734664	75.45%	9.984%
42	9.186	2516	2518	2519	rBV	328	140	0.01%	0.001%
43	9.328	2560	2562	2567	rBV2	478	258	0.01%	0.001%
44	9.376	2575	2577	2578	rBV	368	102	0.00%	0.001%
45	9.537	2625	2627	2629	rBV	642	273	0.01%	0.002%
46	9.556	2629	2633	2637	rVV3	614	709	0.03%	0.004%
47	9.717	2681	2683	2685	rBV2	255	160	0.01%	0.001%
48	9.845	2722	2723	2724	rBV	386	97	0.00%	0.001%
49	9.971	2757	2762	2764	rBV2	707	513	0.02%	0.003%
50	10.074	2790	2794	2795	rBV2	489	274	0.01%	0.002%
51	10.222	2828	2840	2857	rBV	611486	964669	41.96%	5.552%
52	10.553	2940	2943	2945	rBV	807	520	0.02%	0.003%
53	10.659	2974	2976	2978	rBV3	365	214	0.01%	0.001%
54	10.685	2982	2984	2989	rVB3	442	301	0.01%	0.002%
55	10.710	2989	2992	2994	rBV3	342	221	0.01%	0.001%
56	10.749	3002	3004	3007	rVB3	471	279	0.01%	0.002%
57	10.797	3016	3019	3022	rBV2	521	457	0.02%	0.003%
58	10.836	3029	3031	3032	rBV2	382	140	0.01%	0.001%
59	11.170	3133	3135	3138	rBV	800	367	0.02%	0.002%
60	11.254	3150	3161	3182	rBV	1066004	1630332	70.91%	9.384%
61	11.508	3237	3240	3245	rVB2	880	521	0.02%	0.003%
62	11.630	3266	3278	3296	rBV	1028498	1598020	69.51%	9.198%
63	11.951	3374	3378	3380	rBV2	418	286	0.01%	0.002%
64	12.321	3491	3493	3495	rBV	442	237	0.01%	0.001%
65	12.389	3510	3514	3516	rBV3	582	481	0.02%	0.003%
66	13.312	3799	3801	3802	rBV	555	114	0.00%	0.001%
67	13.376	3816	3821	3822	rBV2	506	430	0.02%	0.002%


Sum of corrected areas: 17373839

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121620\
Data File : VV019671.D
Acq On : 16 Dec 2020 13:48
Operator : SY/MD
Sample : L5098-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

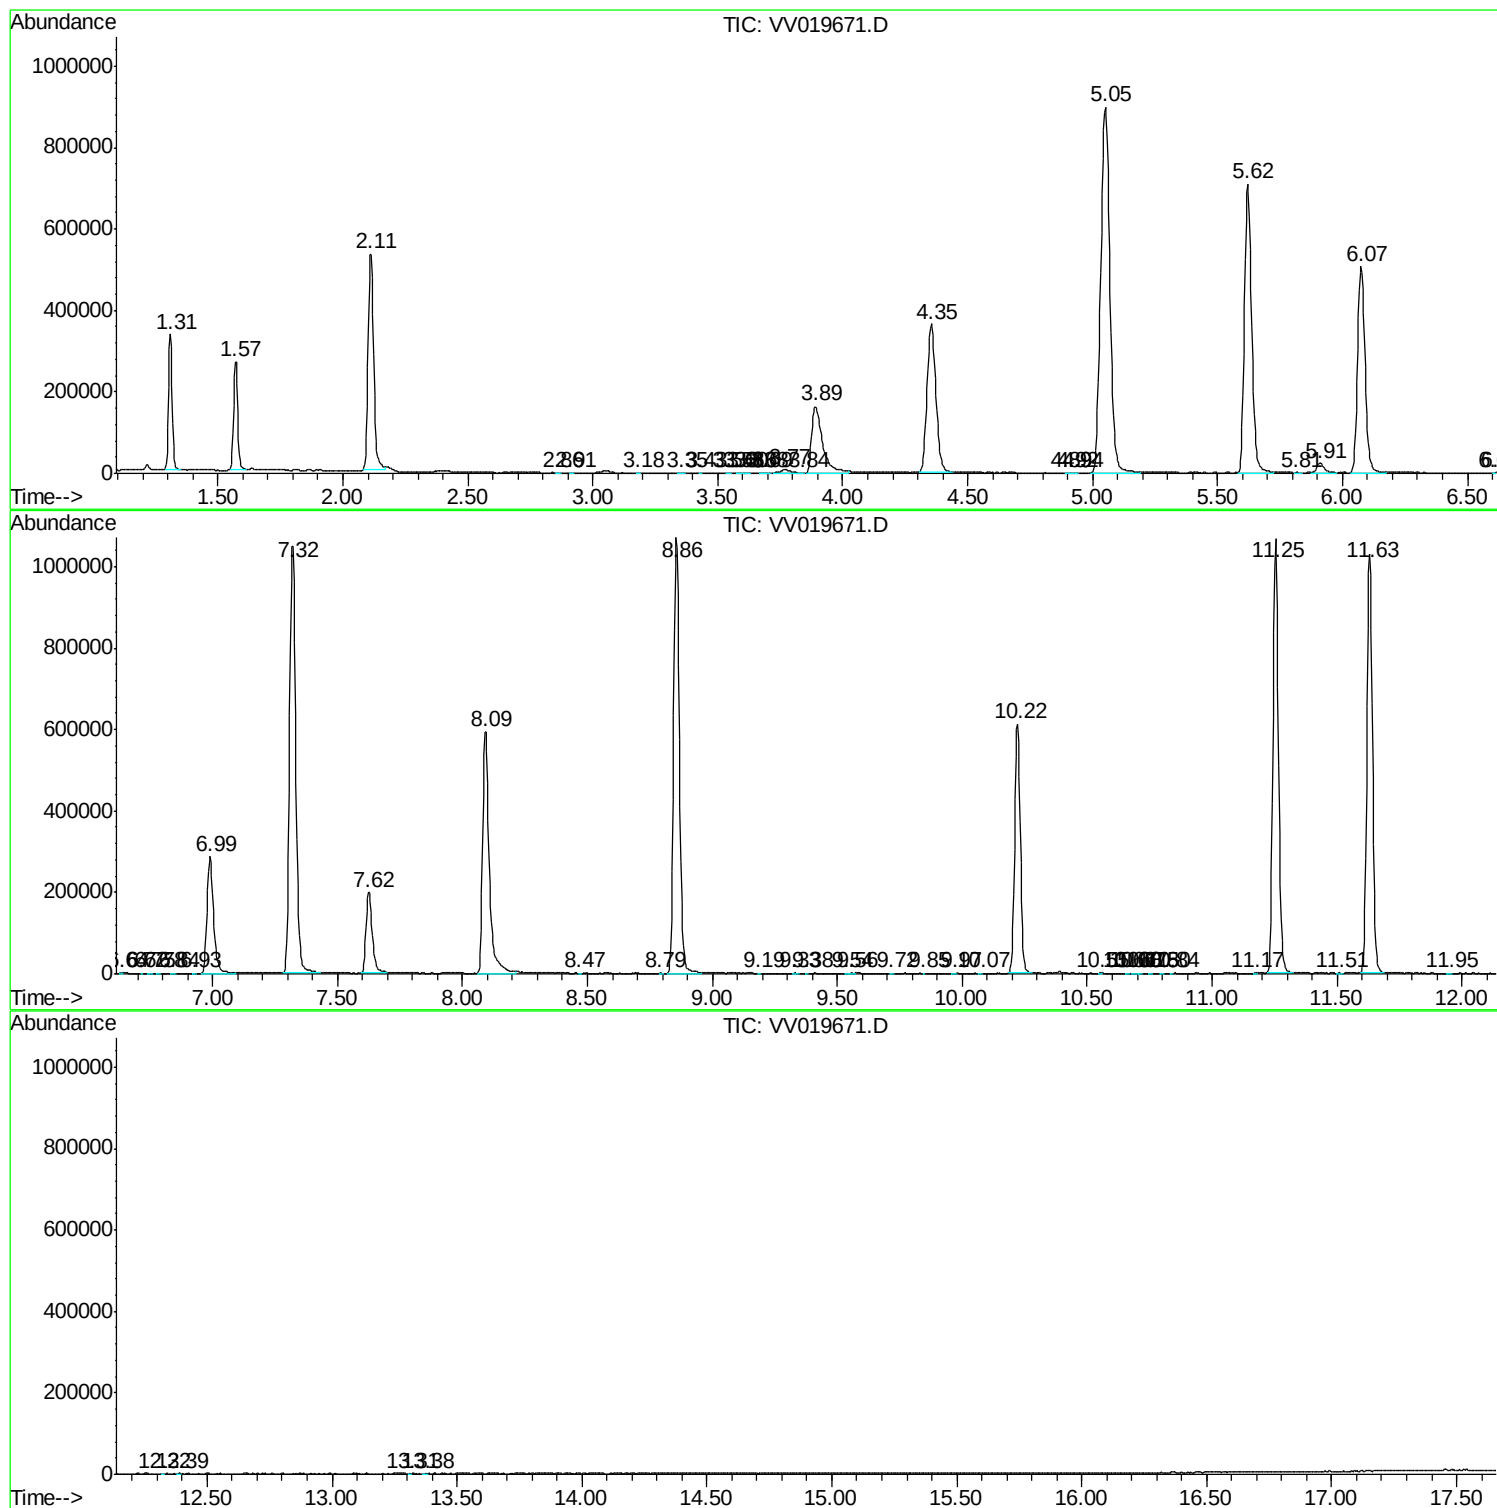

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121620\
Data File : VV019671.D
Acq On : 16 Dec 2020 13:48
Operator : SY/MD
Sample : L5098-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4J1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121620\
Data File : VV019671.D
Acq On : 16 Dec 2020 13:48
Operator : SY/MD
Sample : L5098-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc