


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121620\
 Data File : VV019666.D
 Acq On : 16 Dec 2020 09:33
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 21 06:23:42 2020

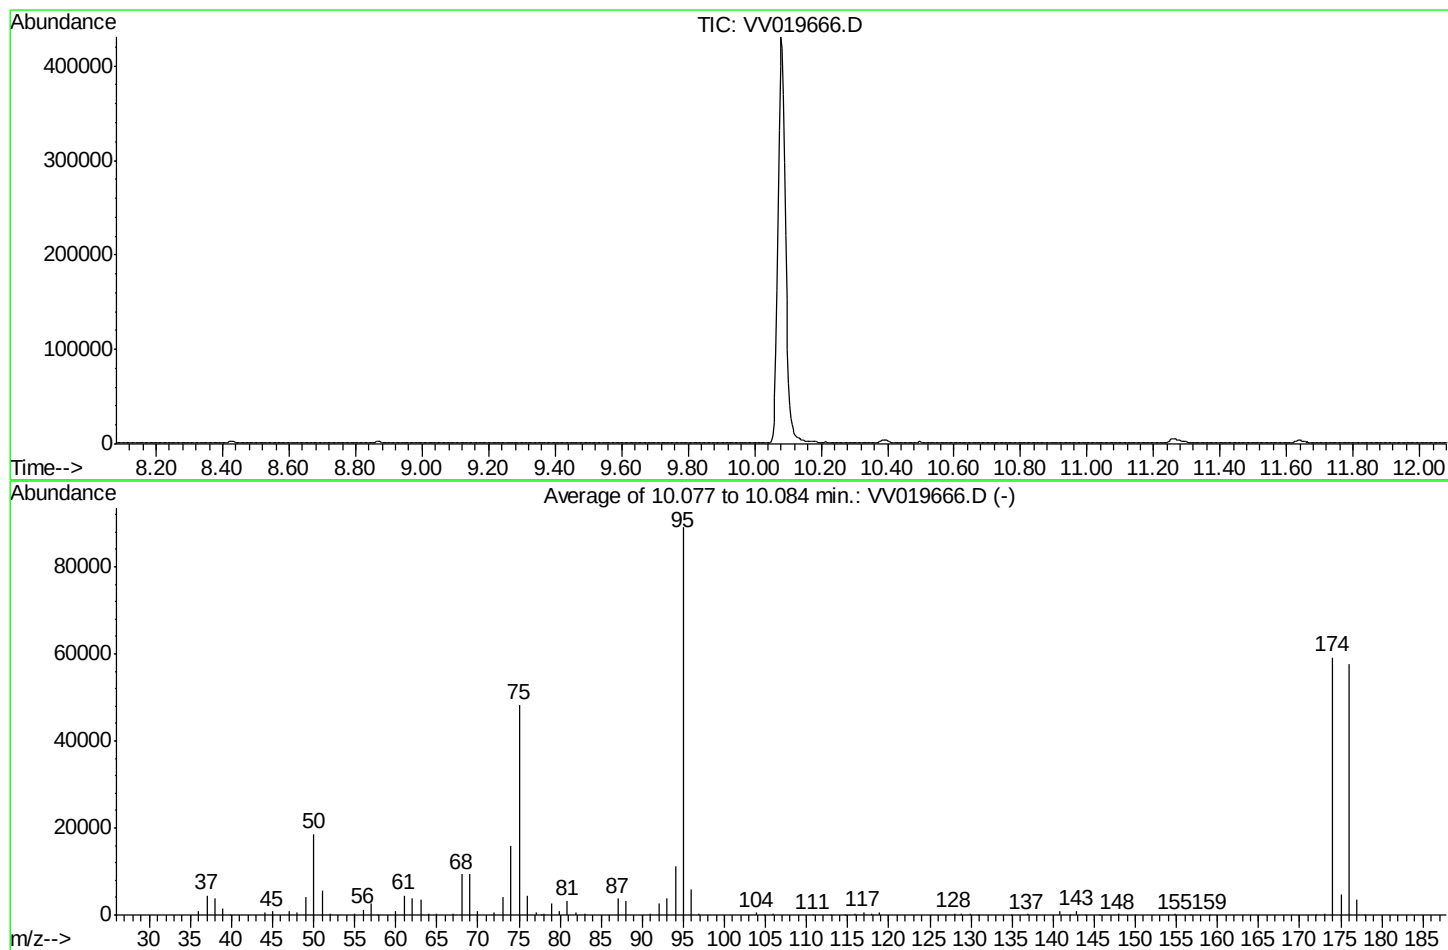

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	18669	PASS
75	95	30	80	54.3	48360	PASS
95	95	100	100	100.0	89042	PASS
96	95	5	9	6.7	6000	PASS
173	174	0.00	2	0.4	220	PASS
174	95	50	120	66.5	59224	PASS
175	174	5	9	8.0	4748	PASS
176	174	95	101	97.5	57773	PASS
177	176	5	9	6.3	3636	PASS

Scan 2784 (10.042 min): VV019666.D
BFB67

m/z	Abundance
38.20	100.0
39.10	114.0
39.90	222.0
44.00	703.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	974.0
37.00	4420.0
38.00	3766.0
39.00	1656.0
39.90	306.0
44.10	1327.0
45.00	792.0
47.00	962.0
47.90	667.0
49.00	3923.0
50.00	17880.0
51.00	5190.0
52.00	252.0
55.00	279.0
56.00	1212.0
57.00	2625.0
57.80	137.0
60.00	976.0
61.00	4520.0
62.00	3788.0
63.00	3563.0
64.00	356.0
65.10	208.0
67.00	393.0
68.00	9155.0
69.00	8988.0
70.00	797.0
71.90	516.0
73.00	3958.0
74.00	15447.0
75.00	46552.0
76.00	4404.0
77.10	556.0
78.00	292.0
78.90	2667.0
79.90	667.0
80.90	3083.0
81.90	614.0
83.00	166.0
87.00	3731.0
87.90	3142.0
91.00	346.0
92.00	2421.0
93.00	3470.0
94.00	10525.0
95.00	86408.0
96.00	5937.0
96.90	182.0
103.90	535.0
104.90	122.0
105.90	402.0
110.80	147.0
115.90	307.0
116.90	533.0
117.90	286.0
118.90	536.0
128.00	347.0
128.90	152.0
129.90	327.0
130.80	102.0
134.80	102.0
136.90	116.0
140.90	728.0
142.00	108.0
142.80	937.0
143.90	136.0
147.90	220.0
150.00	106.0
154.80	136.0
174.00	55816.0
175.00	4605.0
176.00	54504.0
177.00	3439.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	965.0
37.00	4640.0
38.00	4024.0
39.00	1668.0
39.90	341.0
44.00	1373.0
45.00	857.0
47.00	1080.0
47.90	630.0
49.00	4198.0
50.00	19424.0
51.00	5703.0
52.00	287.0
54.90	334.0
56.00	1387.0
57.00	2824.0
57.90	152.0
60.00	991.0
61.00	4756.0
62.00	4025.0
63.00	3735.0
64.00	344.0
65.00	234.0
67.00	425.0
68.00	9615.0
69.00	9555.0
70.00	751.0
71.90	628.0
73.00	4114.0
74.00	16327.0
75.00	50160.0
76.00	4600.0
77.00	569.0
78.10	243.0
78.90	2844.0
79.90	785.0
80.90	3365.0
81.90	640.0
82.90	166.0
87.00	3946.0
88.00	3482.0
90.90	315.0
92.00	2582.0
93.00	3811.0
94.00	11547.0
95.00	91856.0
96.00	6218.0
96.90	184.0
103.90	577.0
104.80	137.0
105.90	417.0
110.80	148.0
115.90	329.0
116.90	656.0
117.90	318.0
118.90	559.0
127.90	377.0
128.80	137.0
129.90	331.0
130.80	158.0
134.90	117.0
136.80	157.0
140.90	843.0
142.00	127.0
142.90	1025.0
143.90	172.0
145.70	113.0
147.90	255.0
149.90	103.0
154.90	187.0
159.10	138.0
173.10	661.0
174.00	61320.0
175.00	4936.0
176.00	59832.0
176.90	3723.0
177.80	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	940.0
37.00	4567.0
38.00	3952.0
39.00	1626.0
39.90	347.0
44.00	1325.0
45.00	876.0
47.00	1051.0
47.90	550.0
49.00	4002.0
50.00	18704.0
51.00	5748.0
52.00	296.0
54.80	367.0
56.00	1373.0
57.00	2625.0
57.90	170.0
60.00	893.0
61.00	4380.0
62.00	3998.0
63.00	3447.0
64.00	328.0
64.90	246.0
66.90	413.0
68.00	9176.0
69.00	9377.0
70.00	733.0
71.90	609.0
73.00	3949.0
74.00	15546.0
75.00	48368.0
76.00	4250.0
77.00	574.0
77.70	164.0
78.90	2738.0
79.90	840.0
80.90	3297.0
81.90	650.0
83.00	156.0
87.00	3699.0
88.00	3422.0
90.90	303.0
92.00	2550.0
93.00	3856.0
94.00	11182.0
95.00	88864.0
96.00	5845.0
96.90	185.0
103.90	508.0
104.80	153.0
105.90	381.0
110.80	134.0
112.90	107.0
114.60	123.0
115.90	330.0
116.90	717.0
117.90	363.0
118.90	472.0
127.90	358.0
128.80	119.0
129.00	118.0
130.00	325.0
130.80	184.0
134.90	122.0
136.90	217.0
140.80	876.0
142.00	144.0
142.90	951.0
143.90	166.0
145.70	127.0
148.00	229.0
149.90	107.0
154.90	223.0
156.70	133.0
159.10	136.0
172.00	284.0
174.00	60536.0
175.00	4703.0
176.00	58984.0
176.90	3746.0
177.80	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67