




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024040.D
Acq On : 17 Dec 2021 02:54
Operator : SY/MD
Sample : M5133-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 05:34:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

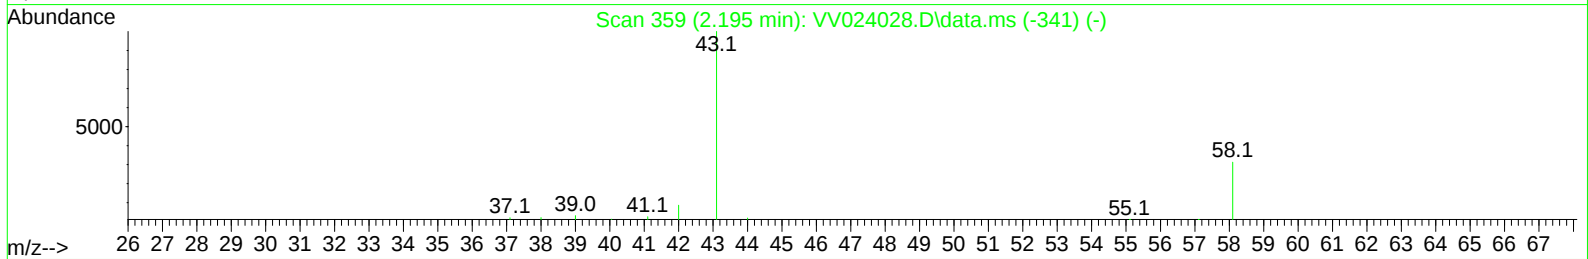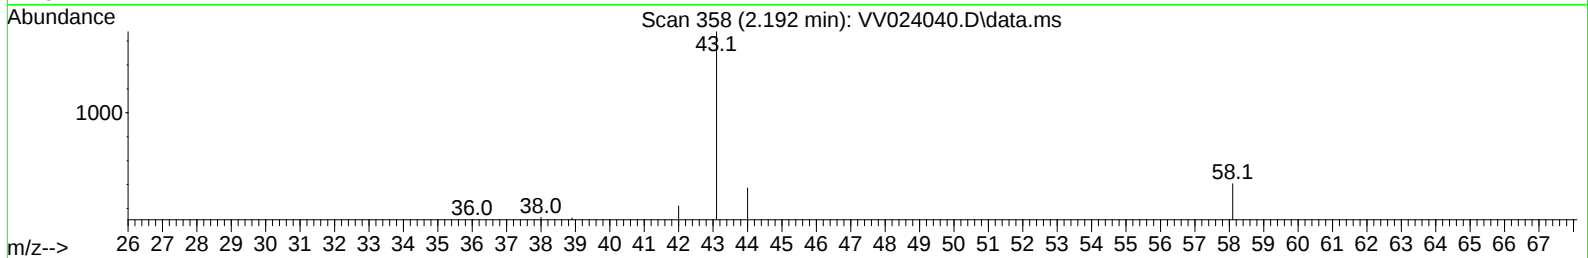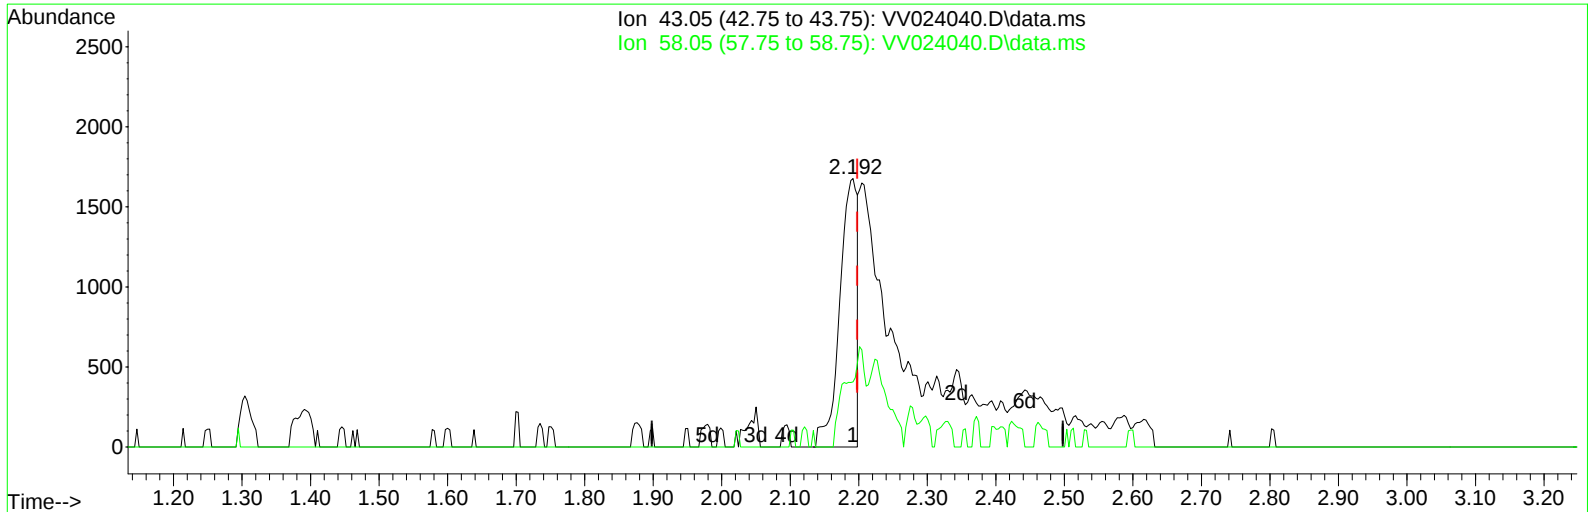

TIC: VV024040.D\data.ms

(13) Acetone (T)

2.192min (-0.006) 3.92 ug/L

response	2981	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	39.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024040.D
Acq On : 17 Dec 2021 02:54
Operator : SY/MD
Sample : M5133-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 05:34:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

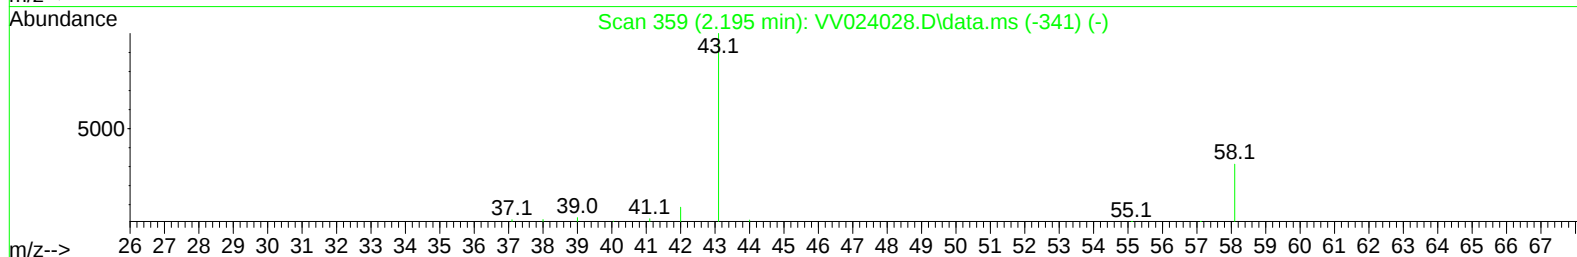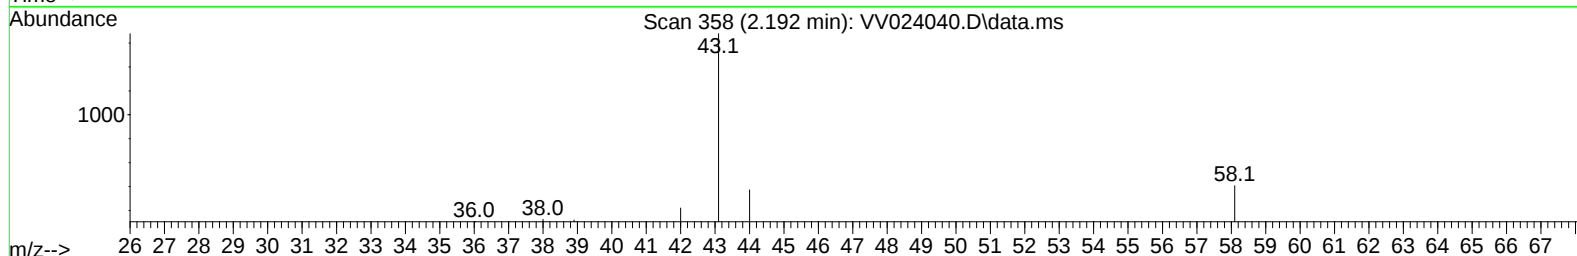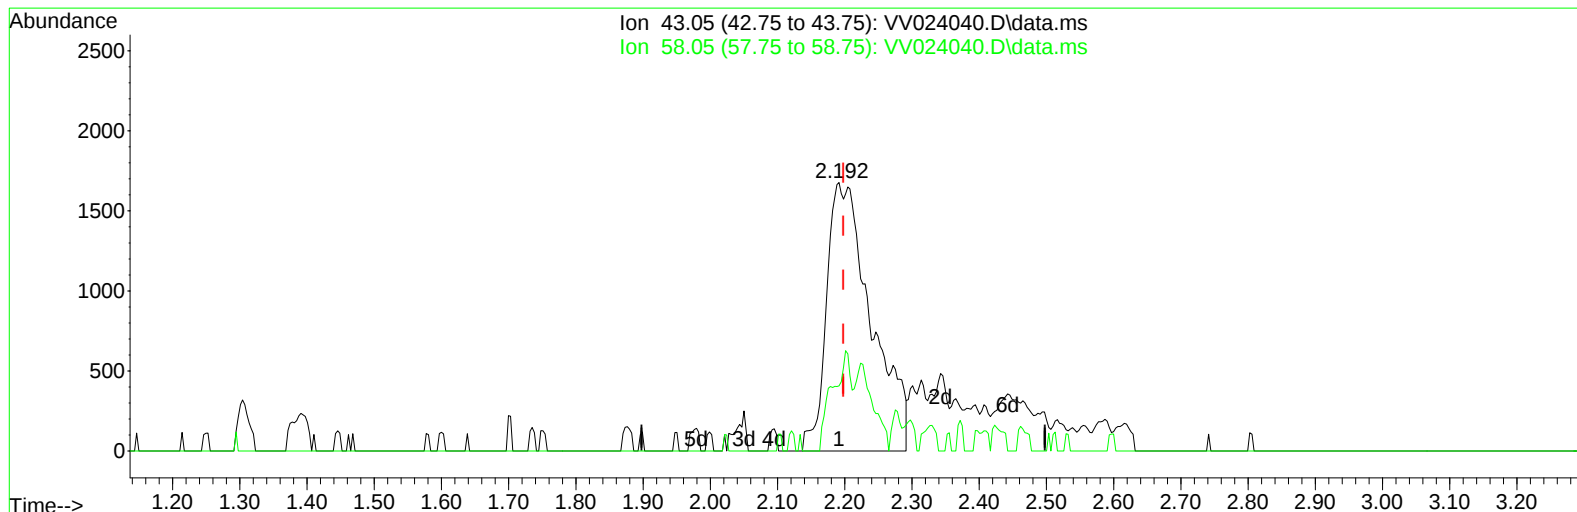

TIC: VV024040.D\data.ms

(13) Acetone (T)

2.192min (-0.006) 10.18 ug/L m

response 7737

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	15.29
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024040.D
 Acq On : 17 Dec 2021 02:54
 Operator : SY/MD
 Sample : M5133-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/17/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 05:34:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	90429	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	95646	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46622	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	24005	4.938	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%
7) Chloroethane-d5	1.565	69	20756	5.117	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.400%
11) 1,1-Dichloroethene-d2	2.105	63	36490	3.845	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.000%
20) 2-Butanone-d5	3.912	46	38068	40.081	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.160%
24) Chloroform-d	4.352	84	52795	4.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.034	65	27549	5.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%
32) Benzene-d6	5.050	84	98244	5.186	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
36) 1,2-Dichloropropane-d6	6.069	67	28824	5.043	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.317	98	88090	5.165	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
43) trans-1,3-Dichloroprop...	7.625	79	10672	4.501	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.092	63	40900	38.533	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.060%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	20501	4.324	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	34900	5.604	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.000%
Target Compounds					Qvalue	
13) Acetone	2.192	43	7737m	10.182	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024040.D
Acq On : 17 Dec 2021 02:54
Operator : SY/MD
Sample : M5133-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 17 05:34:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/22/2021

