

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024004.D
 Acq On : 16 Dec 2021 11:40
 Operator : SY/MD
 Sample : M5090-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D3

Quant Time: Dec 17 02:00:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	89901	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	94499	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46561	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15982	3.307	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.565	69	15619	3.873	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.400%
11) 1,1-Dichloroethene-d2	2.105	63	22570	2.392	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.800%#
20) 2-Butanone-d5	3.889	46	64382	68.185	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	136.380%#
24) Chloroform-d	4.349	84	47697	4.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	5.034	65	23945	4.698	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.050	84	72305	3.863	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.200%
36) 1,2-Dichloropropane-d6	6.069	67	25208	4.464	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.317	98	54184	3.216	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.400%#
43) trans-1,3-Dichloroprop...	7.629	79	8402	3.587	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.800%
46) 2-Hexanone-d5	8.088	63	47365	45.165	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.340%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21605	4.612	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	27935	4.492	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.800%
Target Compounds					Qvalue	
13) Acetone	2.179	43	3577	4.735	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024004.D
Acq On : 16 Dec 2021 11:40
Operator : SY/MD
Sample : M5090-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D3

Quant Time: Dec 17 02:00:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

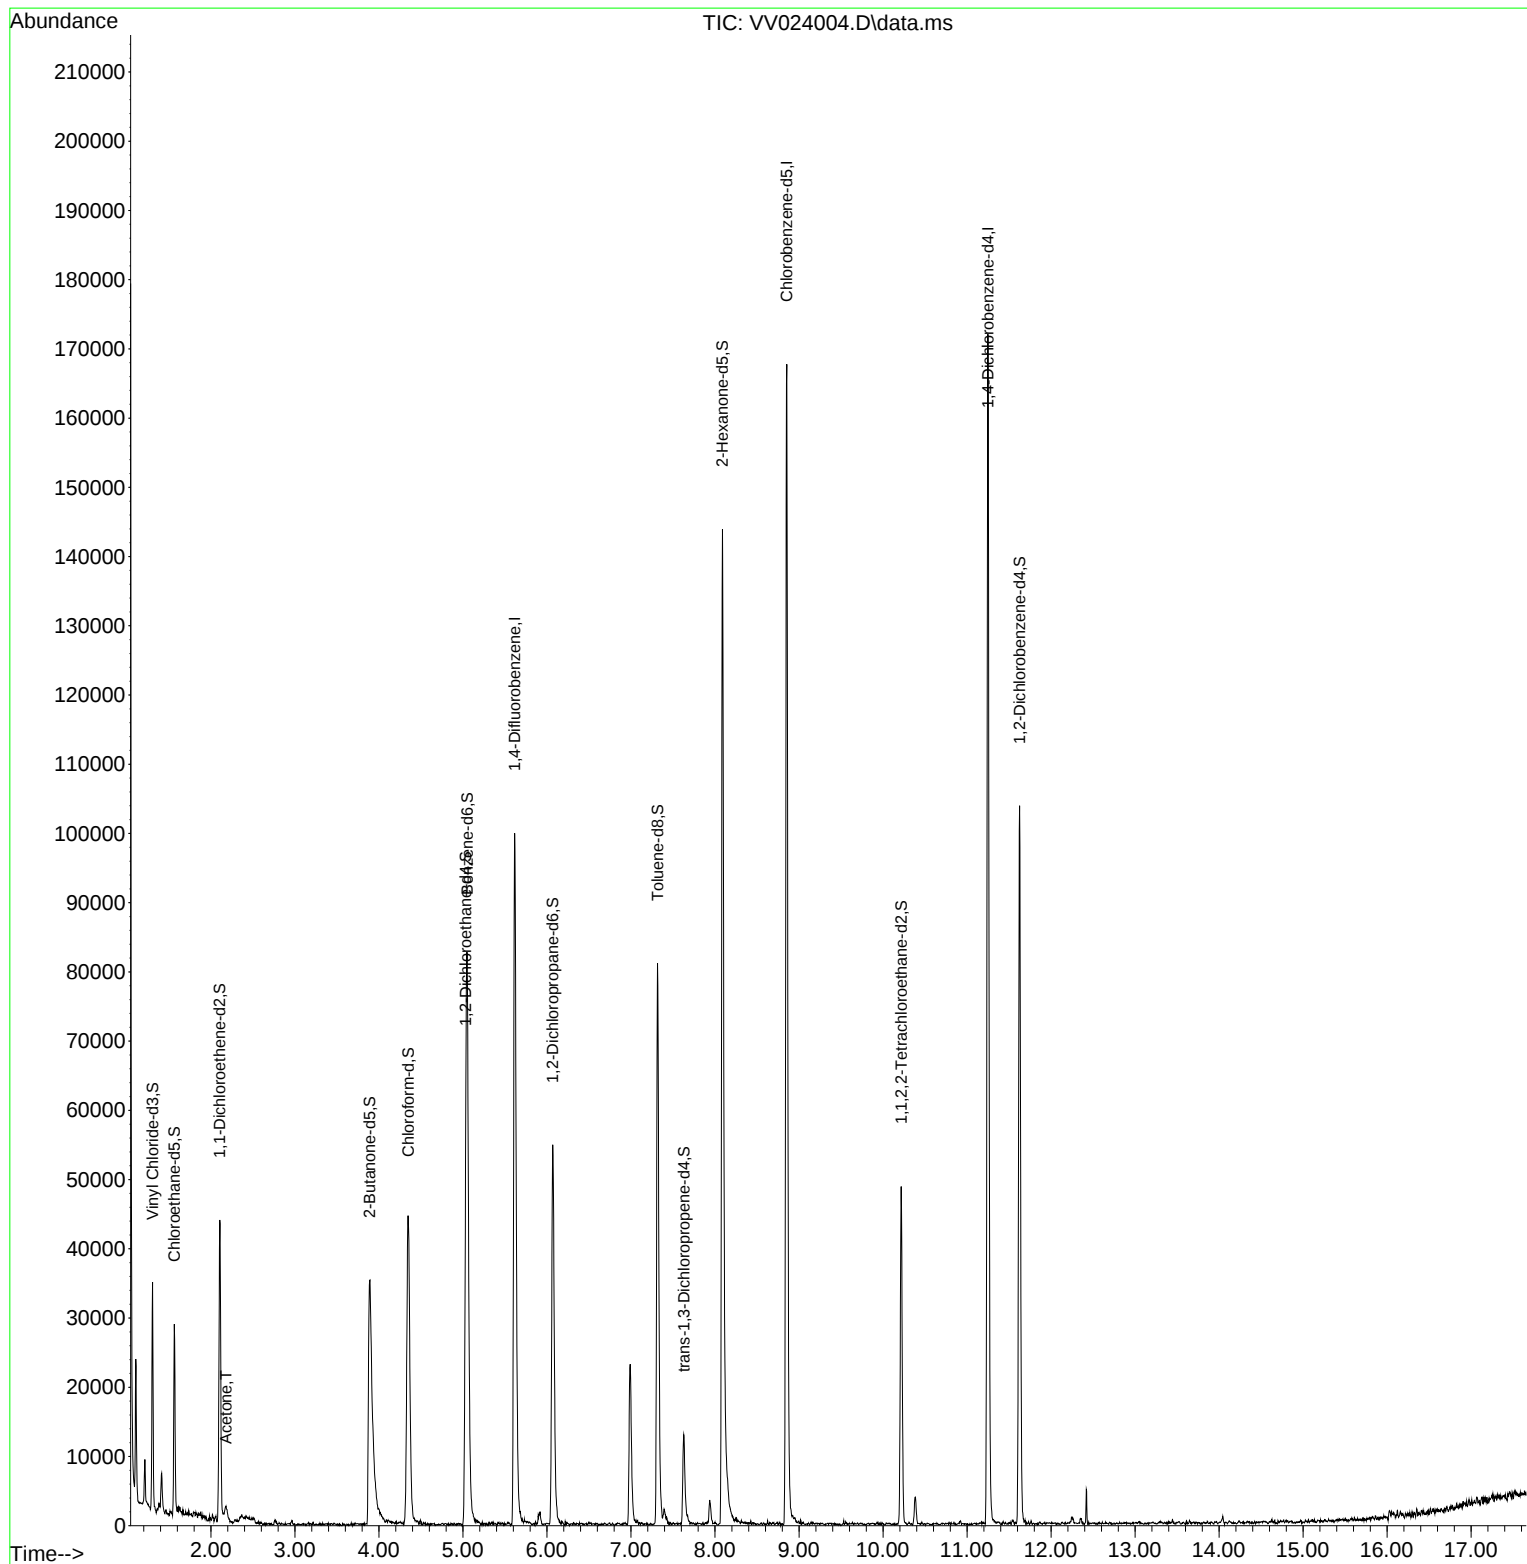

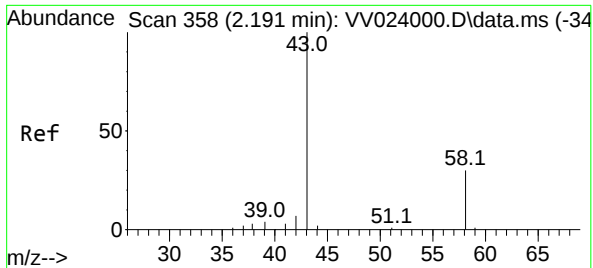

#13
 Acetone
 Concen: 4.735 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV024004.D
 Acq: 16 Dec 2021 11:40

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D3

Tgt Ion: 43 Resp: 3577
 Ion Ratio Lower Upper
 43 100
 58 26.0 0.0 41.4

