

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024007.D
 Acq On : 16 Dec 2021 12:52
 Operator : SY/MD
 Sample : M4971-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Dec 17 02:00:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	91233	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	94740	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47249	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	24195	4.933	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.600%
7) Chloroethane-d5	1.568	69	21742	5.313	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%
11) 1,1-Dichloroethene-d2	2.105	63	37479	3.915	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.200%
20) 2-Butanone-d5	3.905	46	34943	36.467	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.940%
24) Chloroform-d	4.349	84	54454	4.902	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
26) 1,2-Dichloroethane-d4	5.034	65	25632	4.955	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.050	84	99679	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
36) 1,2-Dichloropropane-d6	6.069	67	29296	5.175	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.317	98	88799	5.256	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.200%
43) trans-1,3-Dichloroprop...	7.625	79	10579	4.504	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.092	63	36651	34.860	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.720%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18657	3.973	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	34039	5.393	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	5073	0.634	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024007.D
Acq On : 16 Dec 2021 12:52
Operator : SY/MD
Sample : M4971-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Dec 17 02:00:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

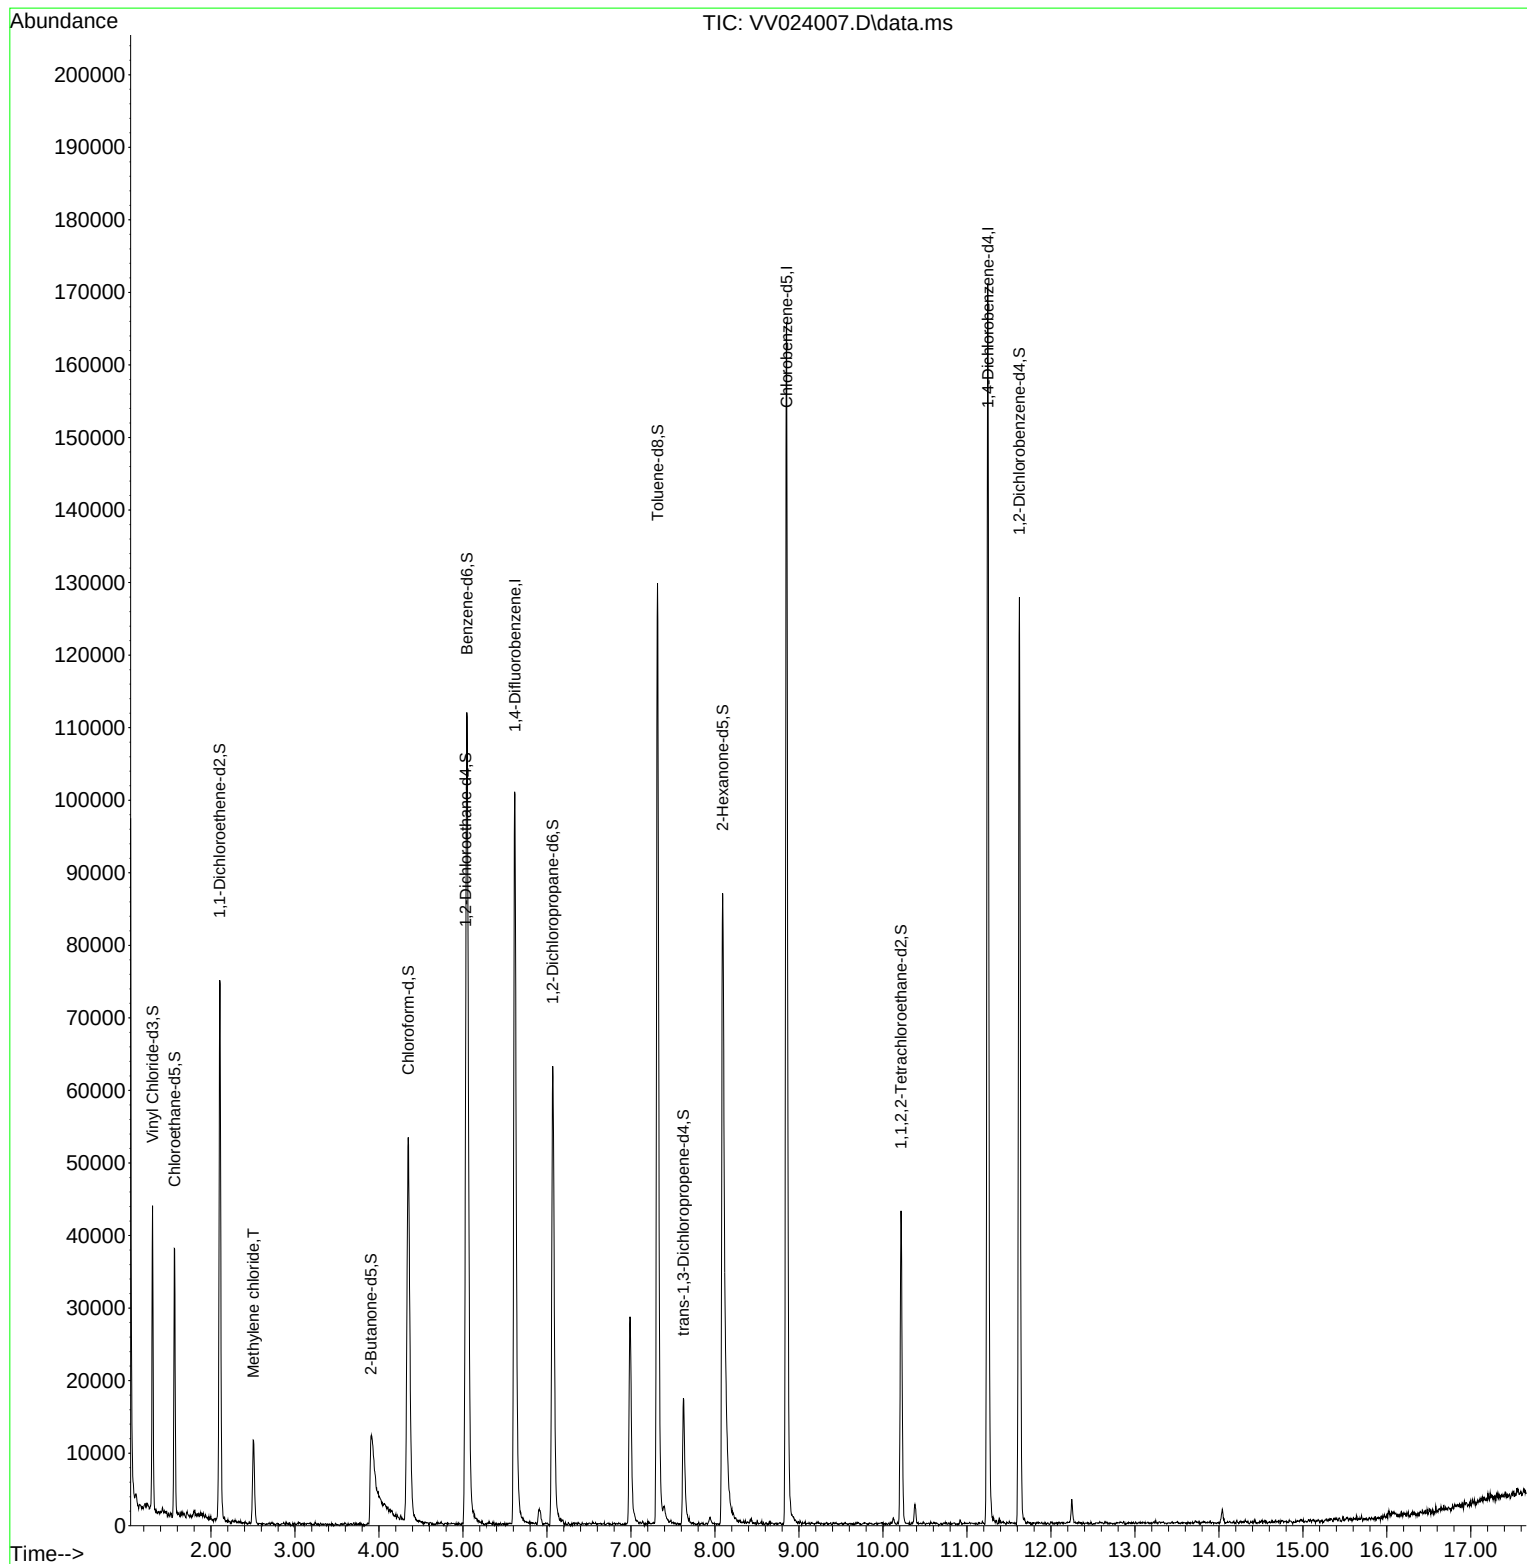

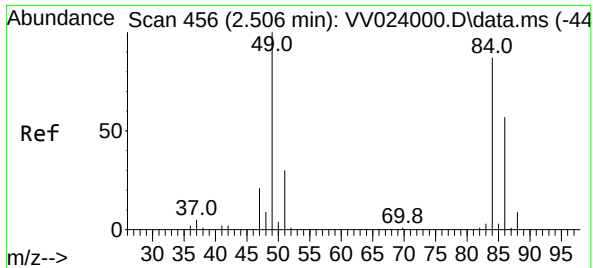

#16
Methylene chloride
Concen: 0.634 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV024007.D
Acq: 16 Dec 2021 12:52

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

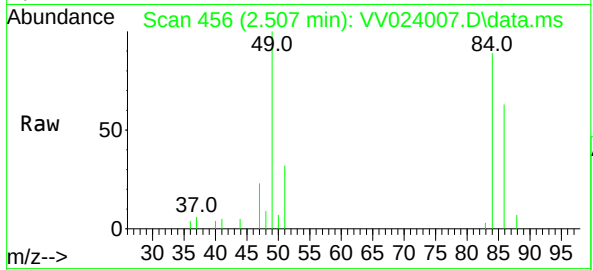

Tgt Ion: 84 Resp: 5073

Ion	Ratio	Lower	Upper
84	100		
86	70.8	42.6	79.0
49	113.0	79.7	147.9

