

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024020.D
 Acq On : 16 Dec 2021 18:02
 Operator : SY/MD
 Sample : M5113-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLU7

Quant Time: Dec 17 02:02:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	93352	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	97765	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49732	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23882	4.759	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.200%
7) Chloroethane-d5	1.568	69	20115	4.804	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.000%
11) 1,1-Dichloroethene-d2	2.108	63	35978	3.673	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	3.895	46	52543	53.590	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.180%
24) Chloroform-d	4.346	84	53551	4.711	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
26) 1,2-Dichloroethane-d4	5.037	65	26941	5.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
32) Benzene-d6	5.050	84	99991	5.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
36) 1,2-Dichloropropane-d6	6.069	67	29107	4.982	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.316	98	89242	5.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.400%
43) trans-1,3-Dichloroprop...	7.628	79	10953	4.519	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.088	63	43197	39.815	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	20594	4.249	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	35956	5.413	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.200%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	15332601	19546.619	ug/L	76
42) Toluene	7.394	91	2832	0.091	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024020.D
Acq On : 16 Dec 2021 18:02
Operator : SY/MD
Sample : M5113-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLU7

Quant Time: Dec 17 02:02:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

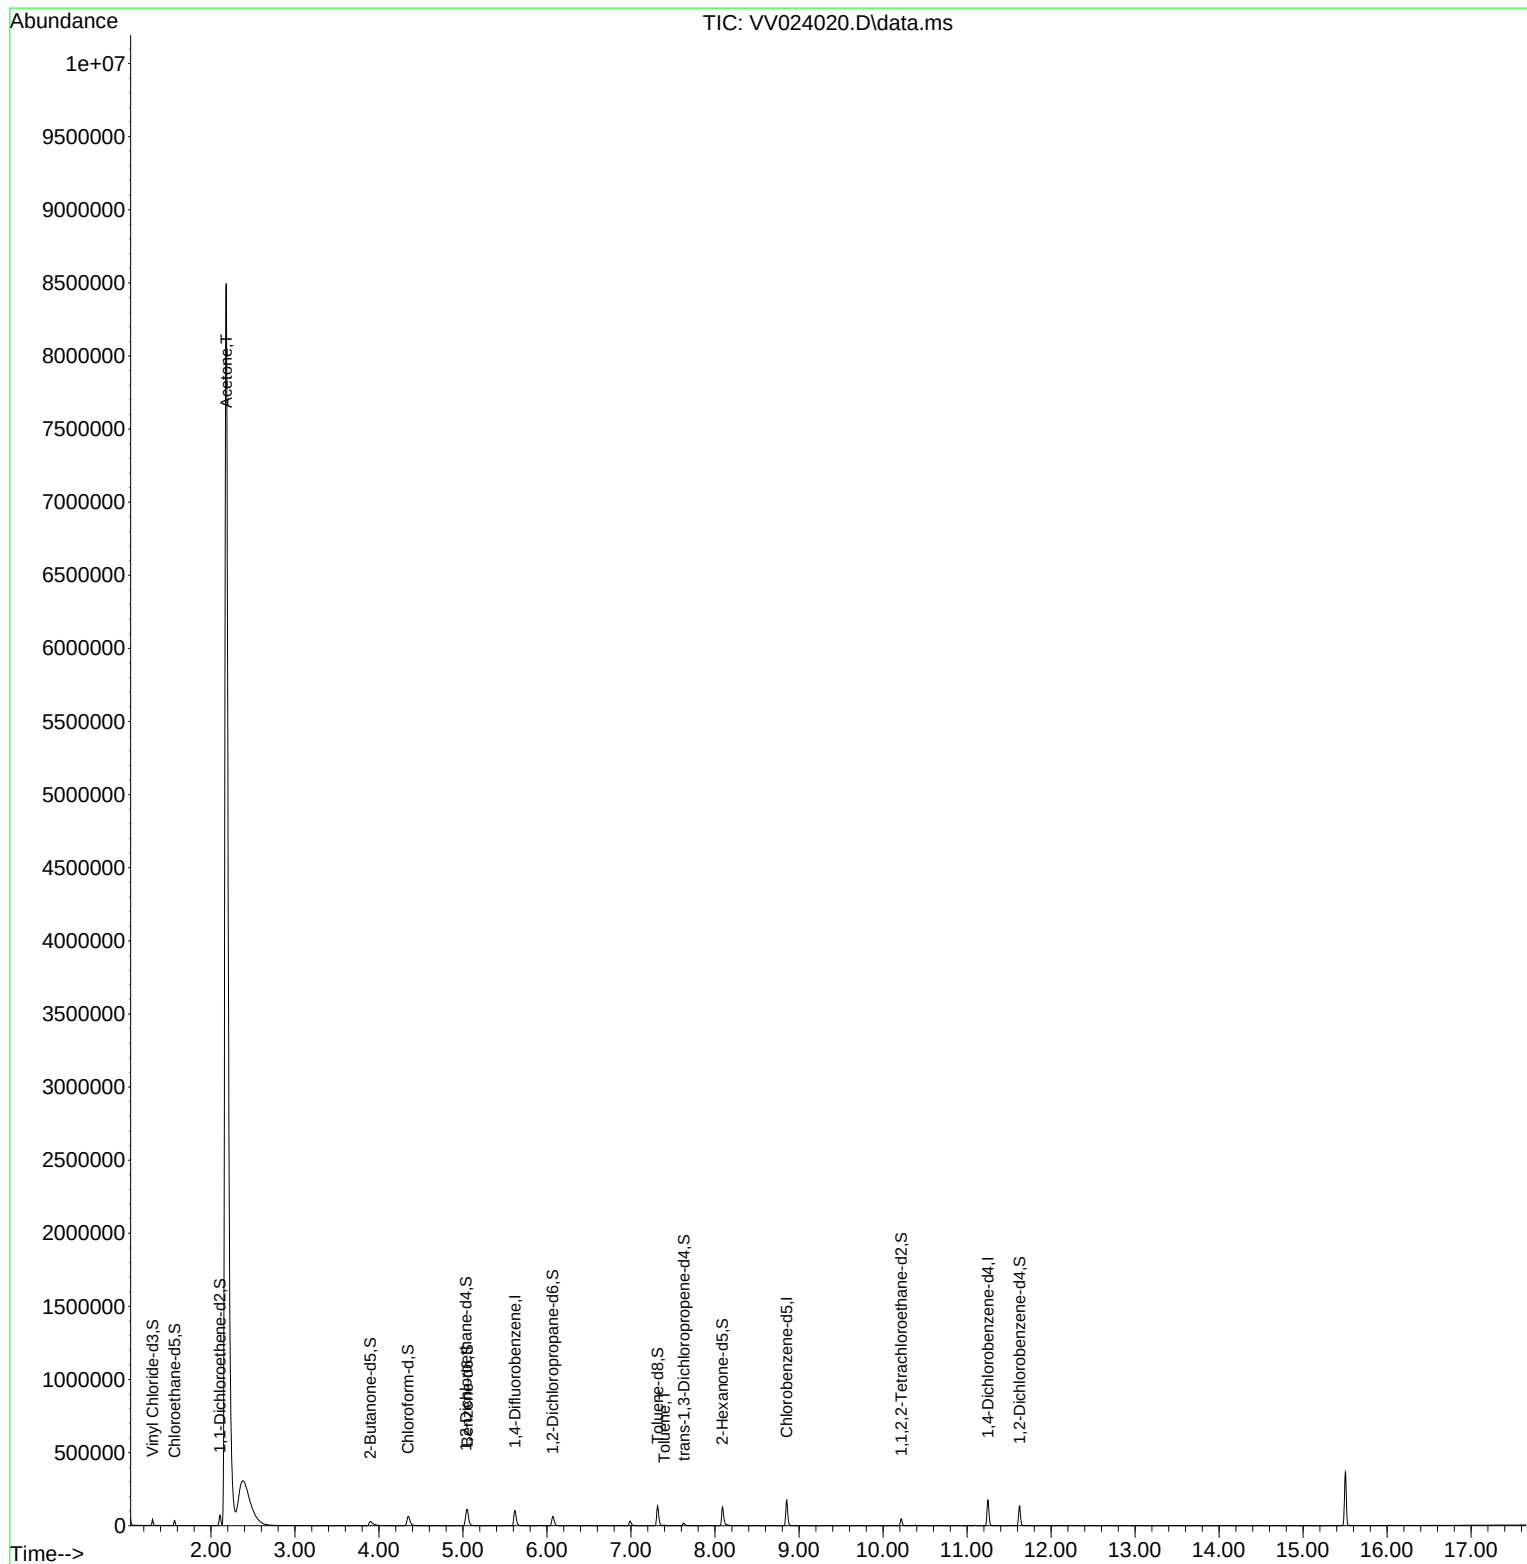

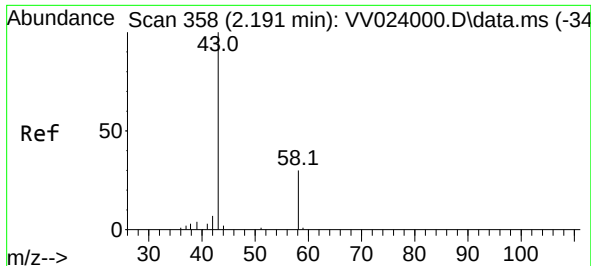

#13

Acetone

Concen: 19546.619 ug/L

RT: 2.182 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV024020.D

Acq: 16 Dec 2021 18:02

Instrument :

MSVOA_V

ClientSampleId :





DBLU7

Tgt Ion: 43 Resp:15332601

Ion Ratio Lower Upper

43 100

58 31.9 0.0 41.4

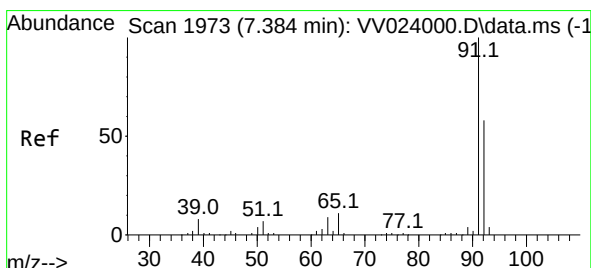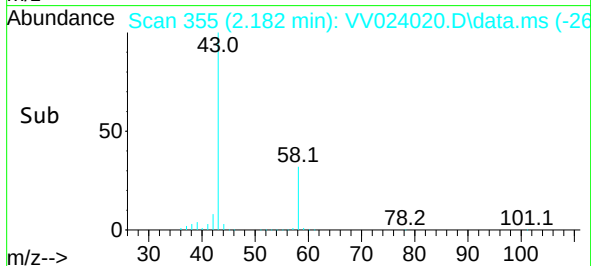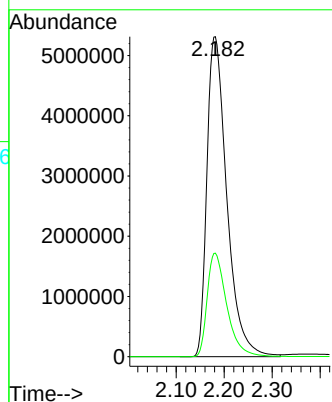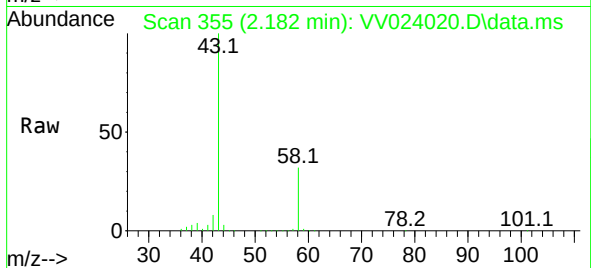

#42

Toluene

Concen: 0.091 ug/L

RT: 7.394 min Scan# 1976

Delta R.T. 0.010 min

Lab File: VV024020.D

Acq: 16 Dec 2021 18:02

Tgt Ion: 91 Resp: 2832

Ion Ratio Lower Upper

91 100

92 74.5 41.5 77.1

