

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
 Data File : VV024029.D
 Acq On : 16 Dec 2021 22:30
 Operator : SY/MD
 Sample : VV1216WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Quant Time: Dec 17 05:32:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	92144	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	98527	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49036	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23701	4.785	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.600%
7) Chloroethane-d5	1.568	69	21078	5.100	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.000%
11) 1,1-Dichloroethene-d2	2.108	63	37017	3.828	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.600%
20) 2-Butanone-d5	3.908	46	39722	41.044	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.080%
24) Chloroform-d	4.349	84	53646	4.781	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.037	65	26592	5.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
32) Benzene-d6	5.050	84	103268	5.292	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.800%
36) 1,2-Dichloropropane-d6	6.069	67	29469	5.005	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.317	98	90676	5.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
43) trans-1,3-Dichloroprop...	7.625	79	10889	4.458	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.091	63	43316	39.616	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.240%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21294	4.360	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	36257	5.535	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%
Target Compounds						
16) Methylene chloride	2.506	84	7199	0.890	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024029.D
Acq On : 16 Dec 2021 22:30
Operator : SY/MD
Sample : VV1216WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Time: Dec 17 05:32:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

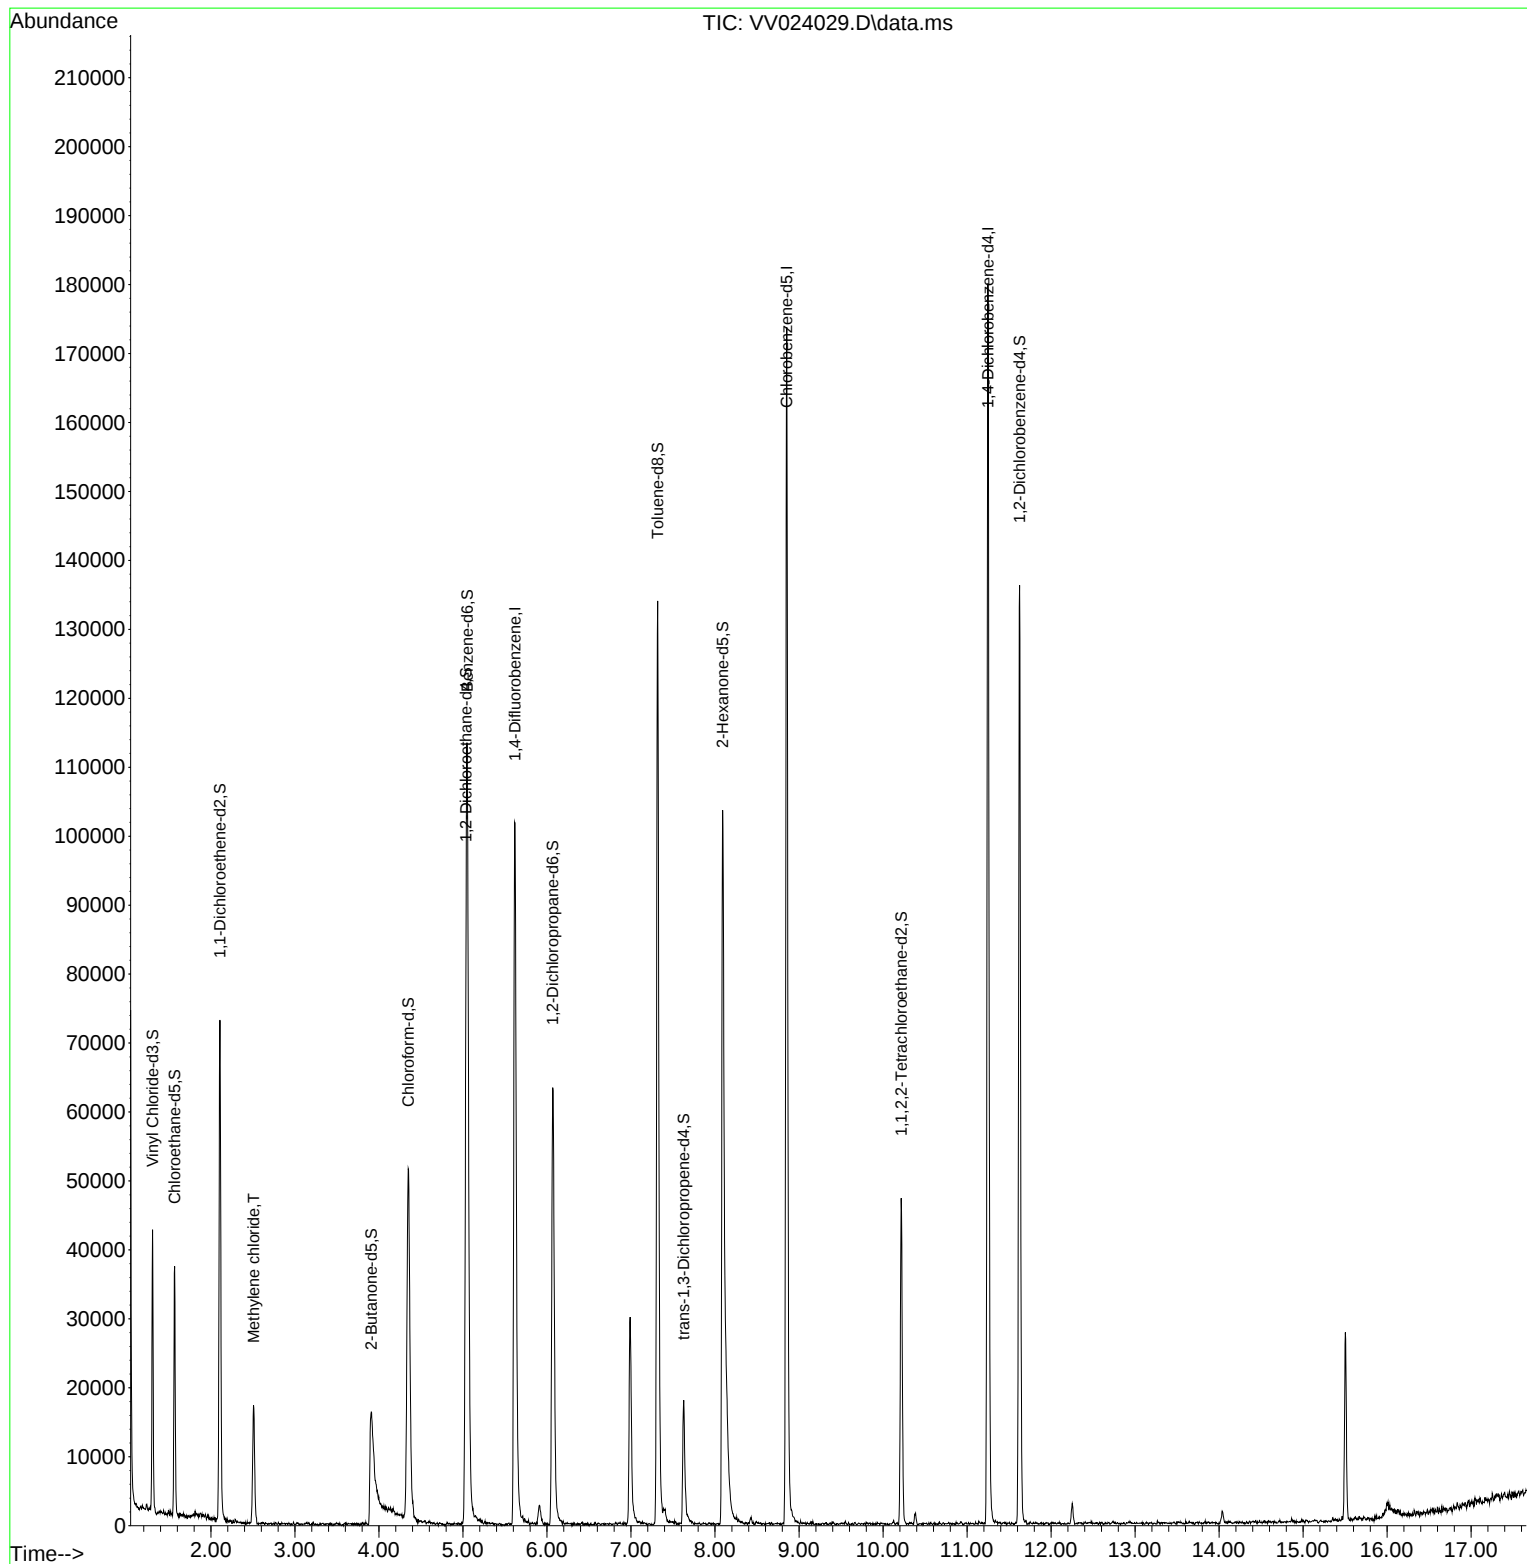

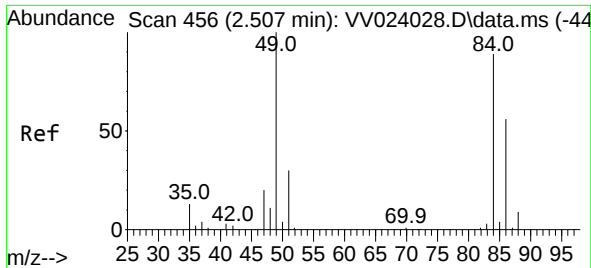

#16
Methylene chloride
Concen: 0.890 ug/L
RT: 2.506 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV024029.D
Acq: 16 Dec 2021 22:30

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Tgt Ion: 84 Resp: 7199
Ion Ratio Lower Upper
84 100
86 67.4 42.6 79.0
49 117.9 79.7 147.9

