

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024033.D
 Acq On : 17 Dec 2021 00:06
 Operator : SY/MD
 Sample : M5133-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH6

Quant Time: Dec 17 05:33:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	91921	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	96395	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48909	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23489	4.753	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.568	69	20123	4.881	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.600%
11) 1,1-Dichloroethene-d2	2.105	63	37105	3.847	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.000%
20) 2-Butanone-d5	3.899	46	42839	44.373	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.740%
24) Chloroform-d	4.349	84	54720	4.889	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.034	65	27736	5.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.400%
32) Benzene-d6	5.050	84	99127	5.192	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
36) 1,2-Dichloropropane-d6	6.069	67	29114	5.054	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.317	98	88757	5.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
43) trans-1,3-Dichloroprop...	7.625	79	10699	4.477	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.091	63	44171	41.291	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.580%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21096	4.415	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	36255	5.549	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.000%
Target Compounds					Qvalue	
13) Acetone	2.191	43	6593	8.536	ug/L	85
31) Carbon tetrachloride	4.828	117	89335	7.536	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024033.D
Acq On : 17 Dec 2021 00:06
Operator : SY/MD
Sample : M5133-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBH6

Quant Time: Dec 17 05:33:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

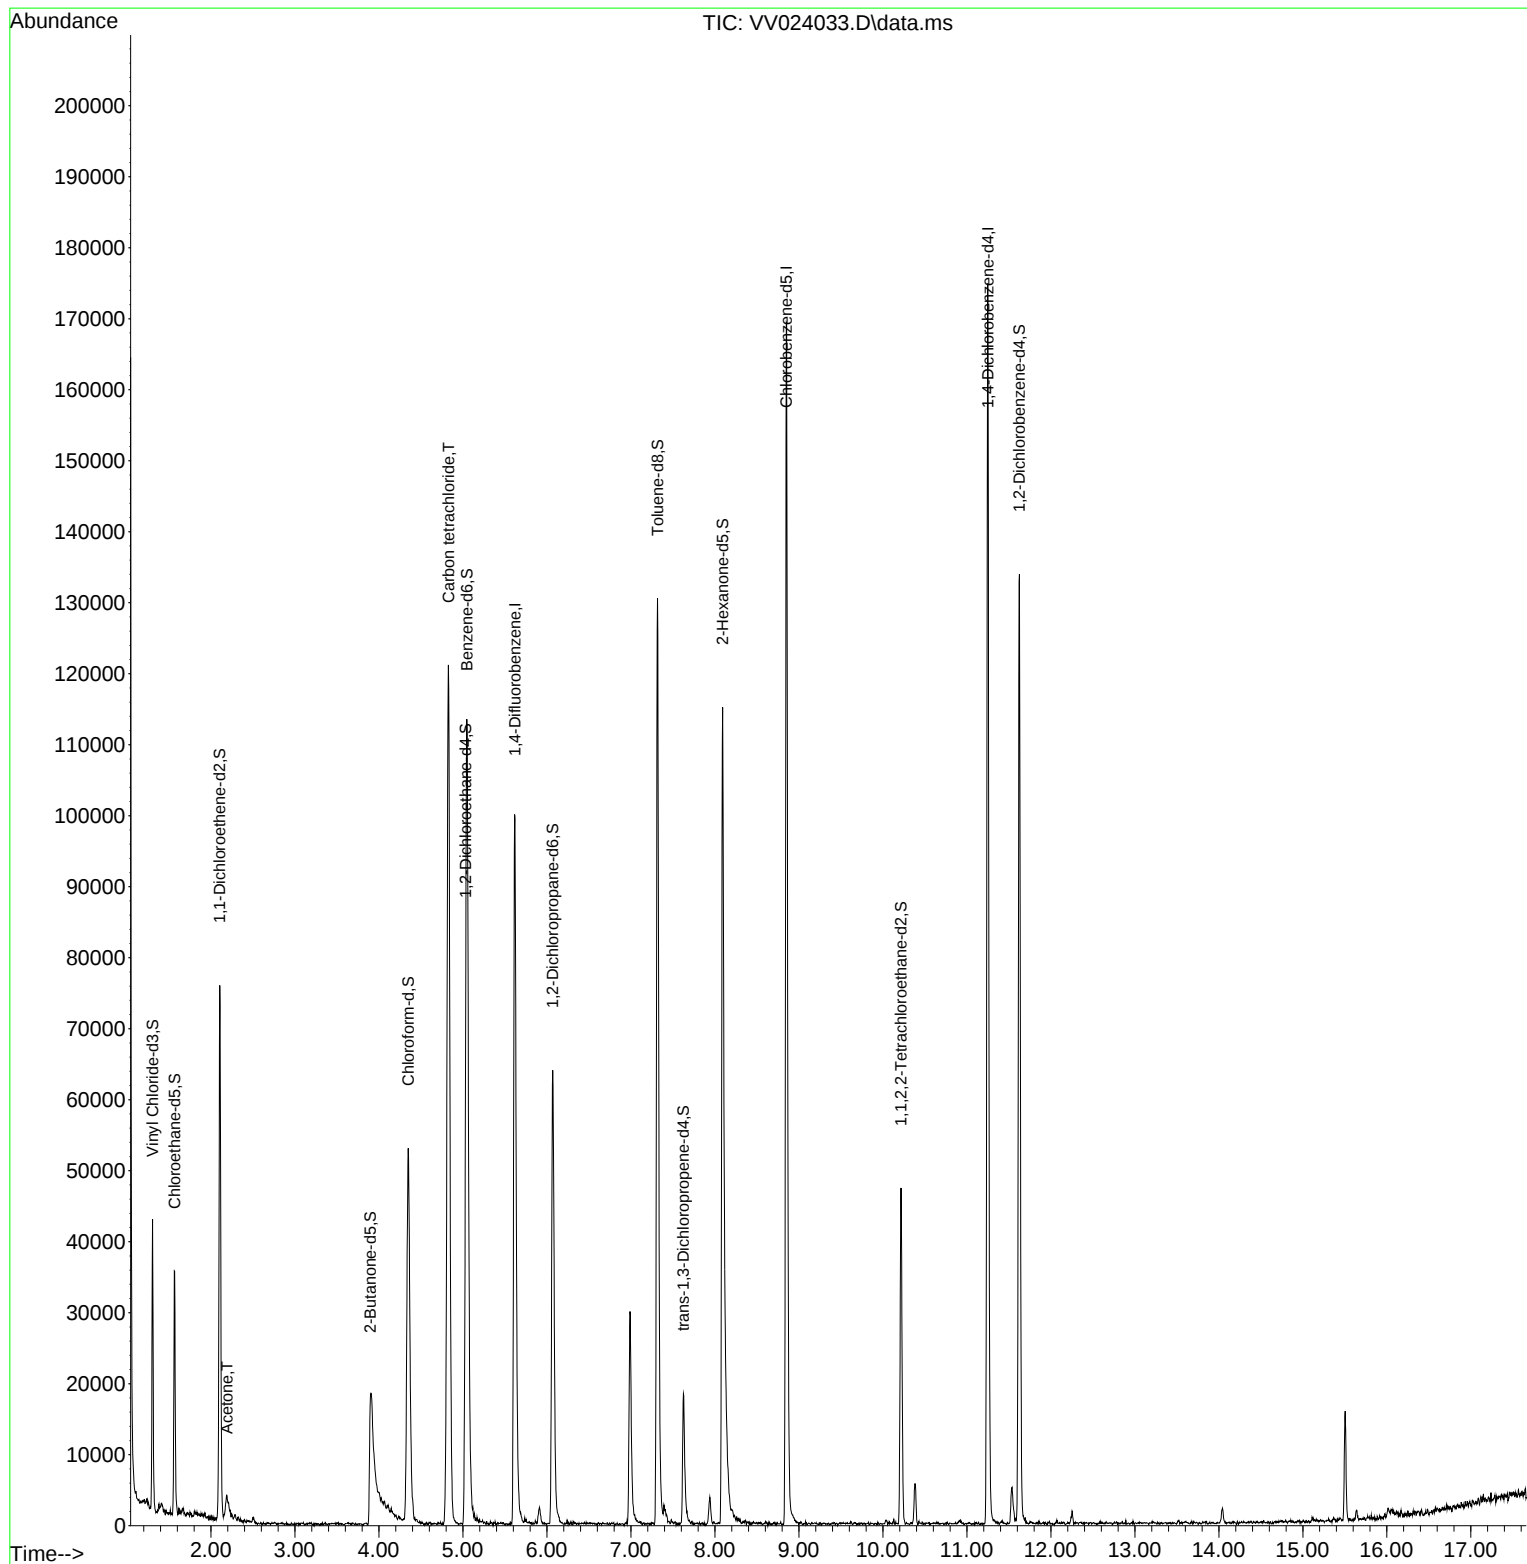

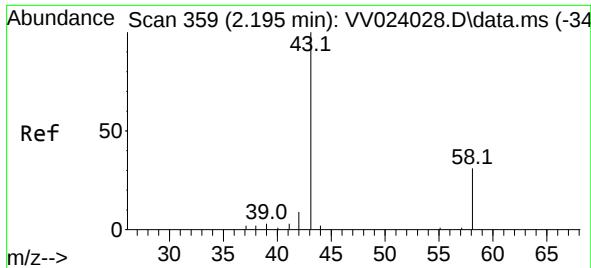

#13

Acetone

Concen: 8.536 ug/L

RT: 2.191 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV024033.D

Acq: 17 Dec 2021 00:06

Instrument :

MSVOA_V

ClientSampleId :





GBBH6

Tgt Ion: 43 Resp: 6593

Ion Ratio Lower Upper

43 100

58 27.7 0.0 41.4

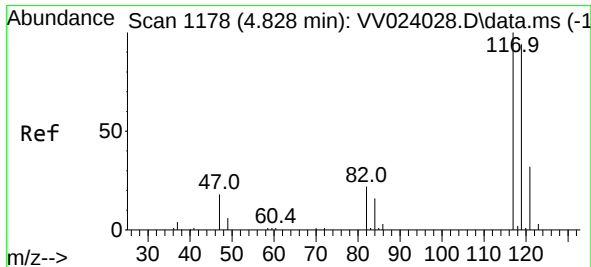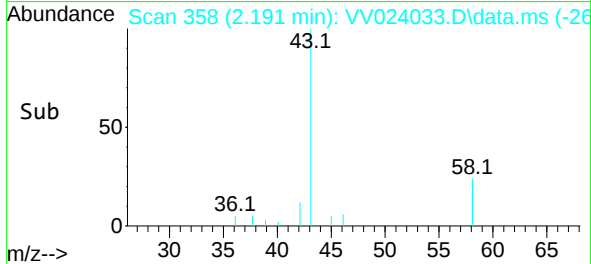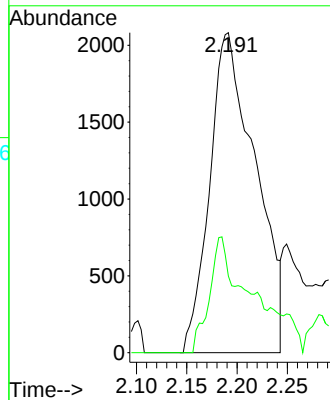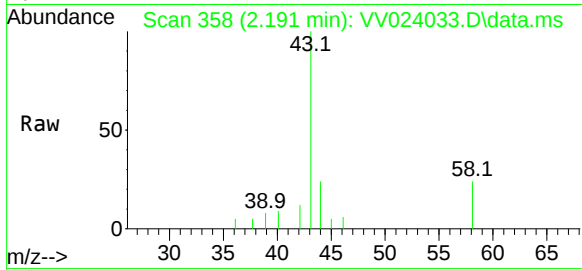

#31

Carbon tetrachloride

Concen: 7.536 ug/L

RT: 4.828 min Scan# 1178

Delta R.T. 0.003 min

Lab File: VV024033.D

Acq: 17 Dec 2021 00:06

Tgt Ion: 117 Resp: 89335

Ion Ratio Lower Upper

117 100

119 96.7 76.6 114.8

