

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VV024034.D
 Acq On : 17 Dec 2021 00:30
 Operator : SY/MD
 Sample : M5133-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH7

Quant Time: Dec 17 05:33:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	91126	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	97763	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49038	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23275	4.751	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.568	69	21415	5.239	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.800%
11) 1,1-Dichloroethene-d2	2.108	63	36994	3.869	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.400%
20) 2-Butanone-d5	3.899	46	54058	56.482	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.960%
24) Chloroform-d	4.349	84	54459	4.908	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.034	65	27228	5.270	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	5.053	84	99367	5.132	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
36) 1,2-Dichloropropane-d6	6.069	67	29385	5.030	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.600%
41) Toluene-d8	7.317	98	90473	5.190	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
43) trans-1,3-Dichloroprop...	7.625	79	10444	4.309	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.088	63	41109	37.891	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.780%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	20753	4.282	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	35836	5.471	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						Qvalue
13) Acetone	2.188	43	9558	12.483	ug/L	77
31) Carbon tetrachloride	4.828	117	31725	2.639	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024034.D
Acq On : 17 Dec 2021 00:30
Operator : SY/MD
Sample : M5133-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBH7

Quant Time: Dec 17 05:33:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

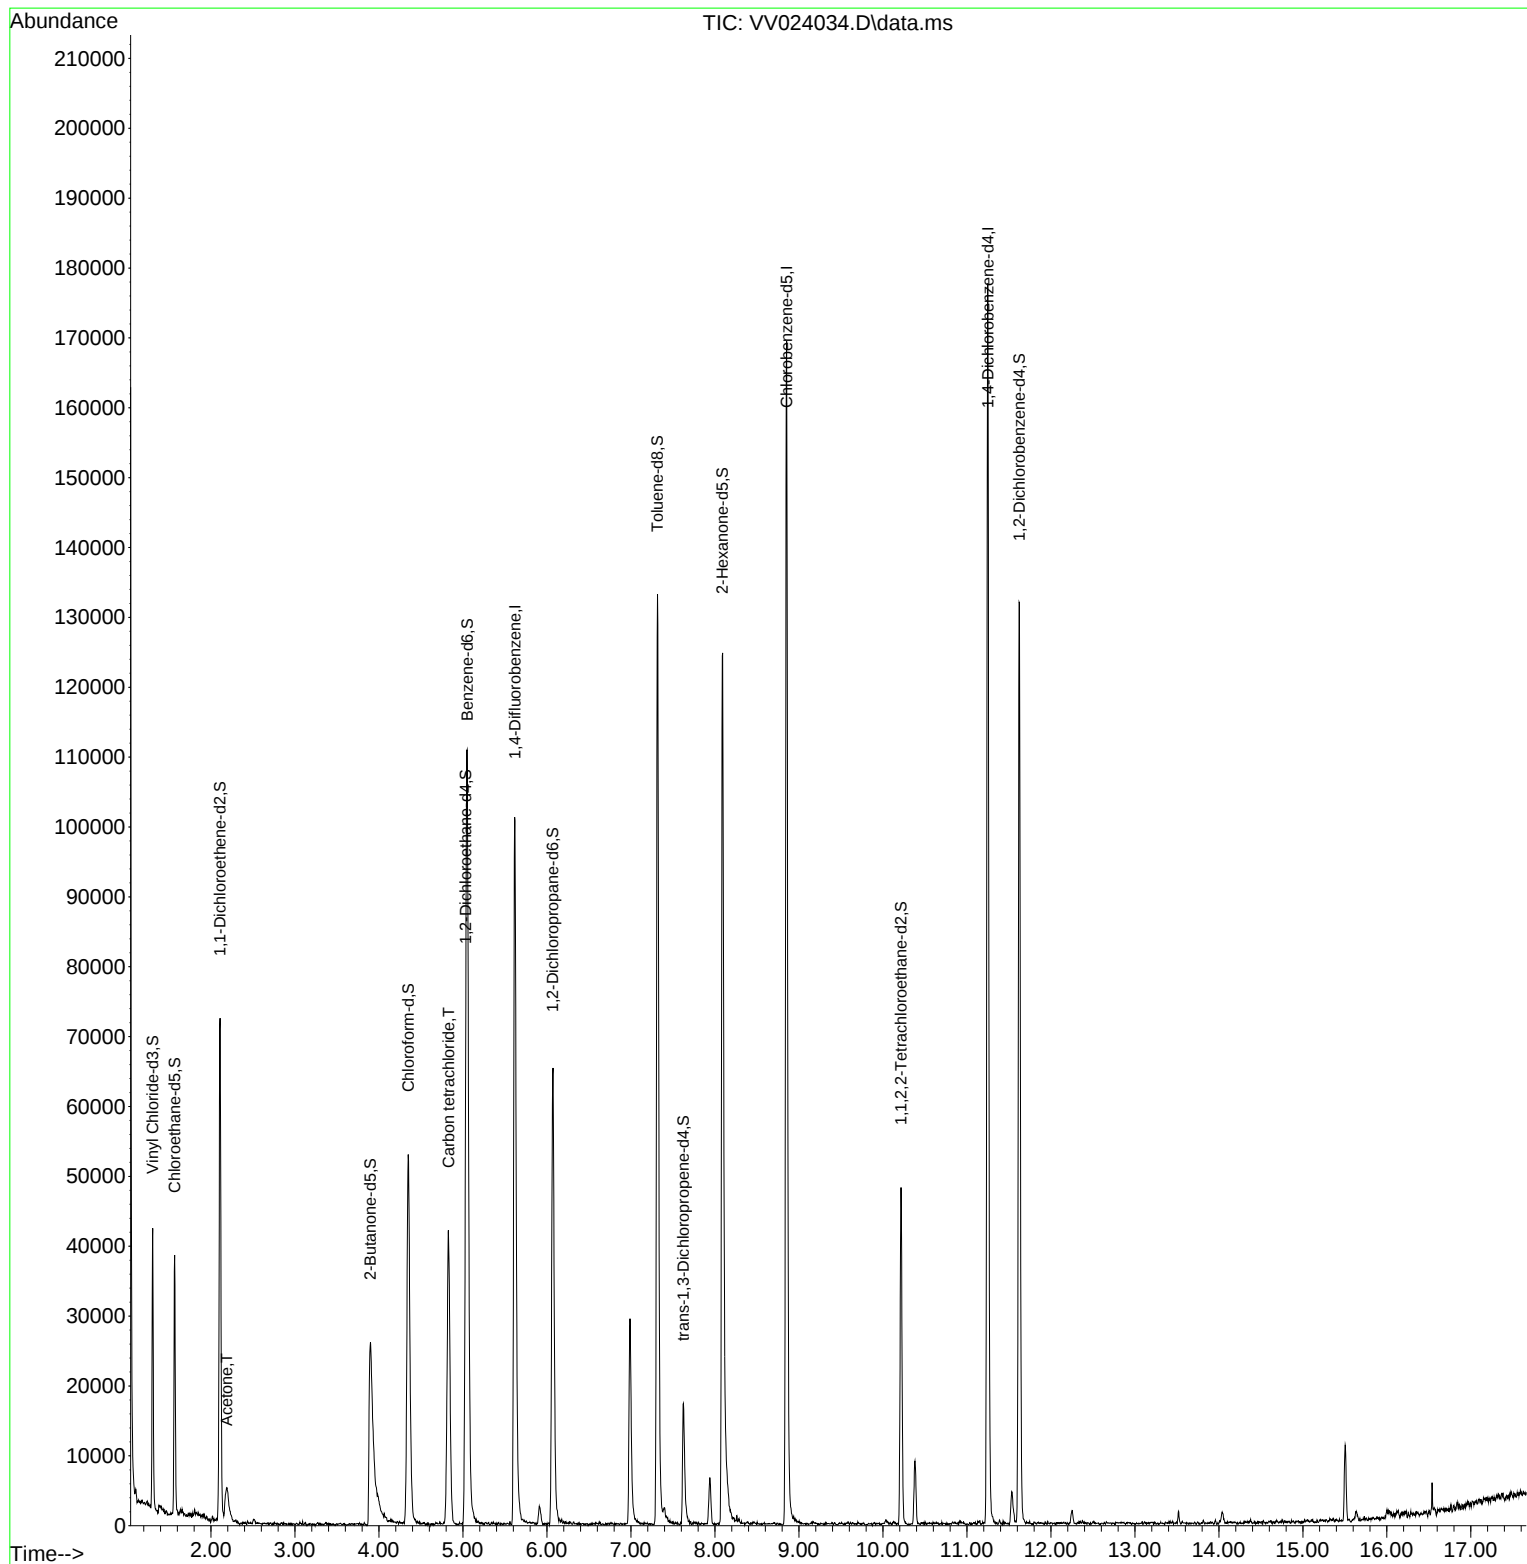

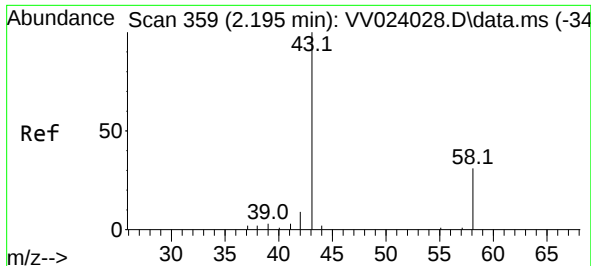

#13

Acetone

Concen: 12.483 ug/L

RT: 2.188 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV024034.D

Acq: 17 Dec 2021 00:30

Instrument :

MSVOA_V

ClientSampleId :





GBBH7

Tgt Ion: 43 Resp: 9558

Ion Ratio Lower Upper

43 100

58 31.3 0.0 41.4

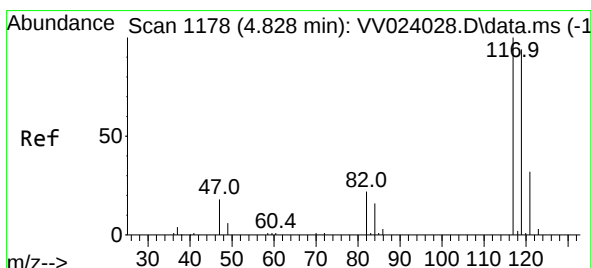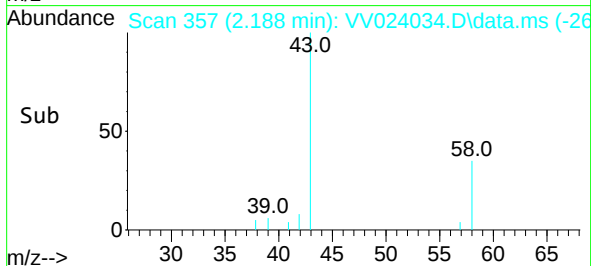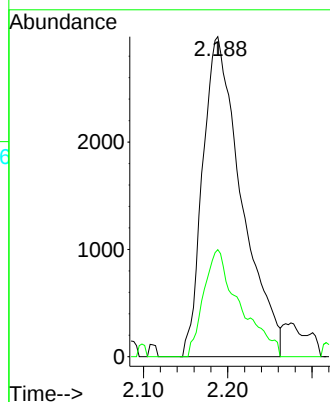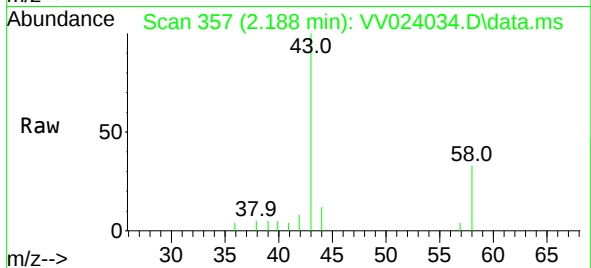

#31

Carbon tetrachloride

Concen: 2.639 ug/L

RT: 4.828 min Scan# 1178

Delta R.T. 0.003 min

Lab File: VV024034.D

Acq: 17 Dec 2021 00:30

Tgt Ion: 117 Resp: 31725

Ion Ratio Lower Upper

117 100

119 94.3 76.6 114.8

