

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024038.D
 Acq On : 17 Dec 2021 02:06
 Operator : SY/MD
 Sample : M5133-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ1

Quant Time: Dec 17 05:34:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	91763	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	99424	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47828	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23421	4.748	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.568	69	20395	4.955	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.108	63	36402	3.780	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	3.902	46	44539	46.213	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.420%
24) Chloroform-d	4.349	84	52382	4.688	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	5.034	65	26339	5.063	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.050	84	96038	4.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	6.072	67	29163	4.909	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%
41) Toluene-d8	7.317	98	86152	4.859	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
43) trans-1,3-Dichloroprop...	7.625	79	10272	4.168	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.400%
46) 2-Hexanone-d5	8.092	63	40713	36.899	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.800%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	19882	4.034	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	34376	5.381	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds						Qvalue
13) Acetone	2.185	43	6488	8.414	ug/L	98
31) Carbon tetrachloride	4.828	117	447110	36.566	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024038.D
Acq On : 17 Dec 2021 02:06
Operator : SY/MD
Sample : M5133-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ1

Quant Time: Dec 17 05:34:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration




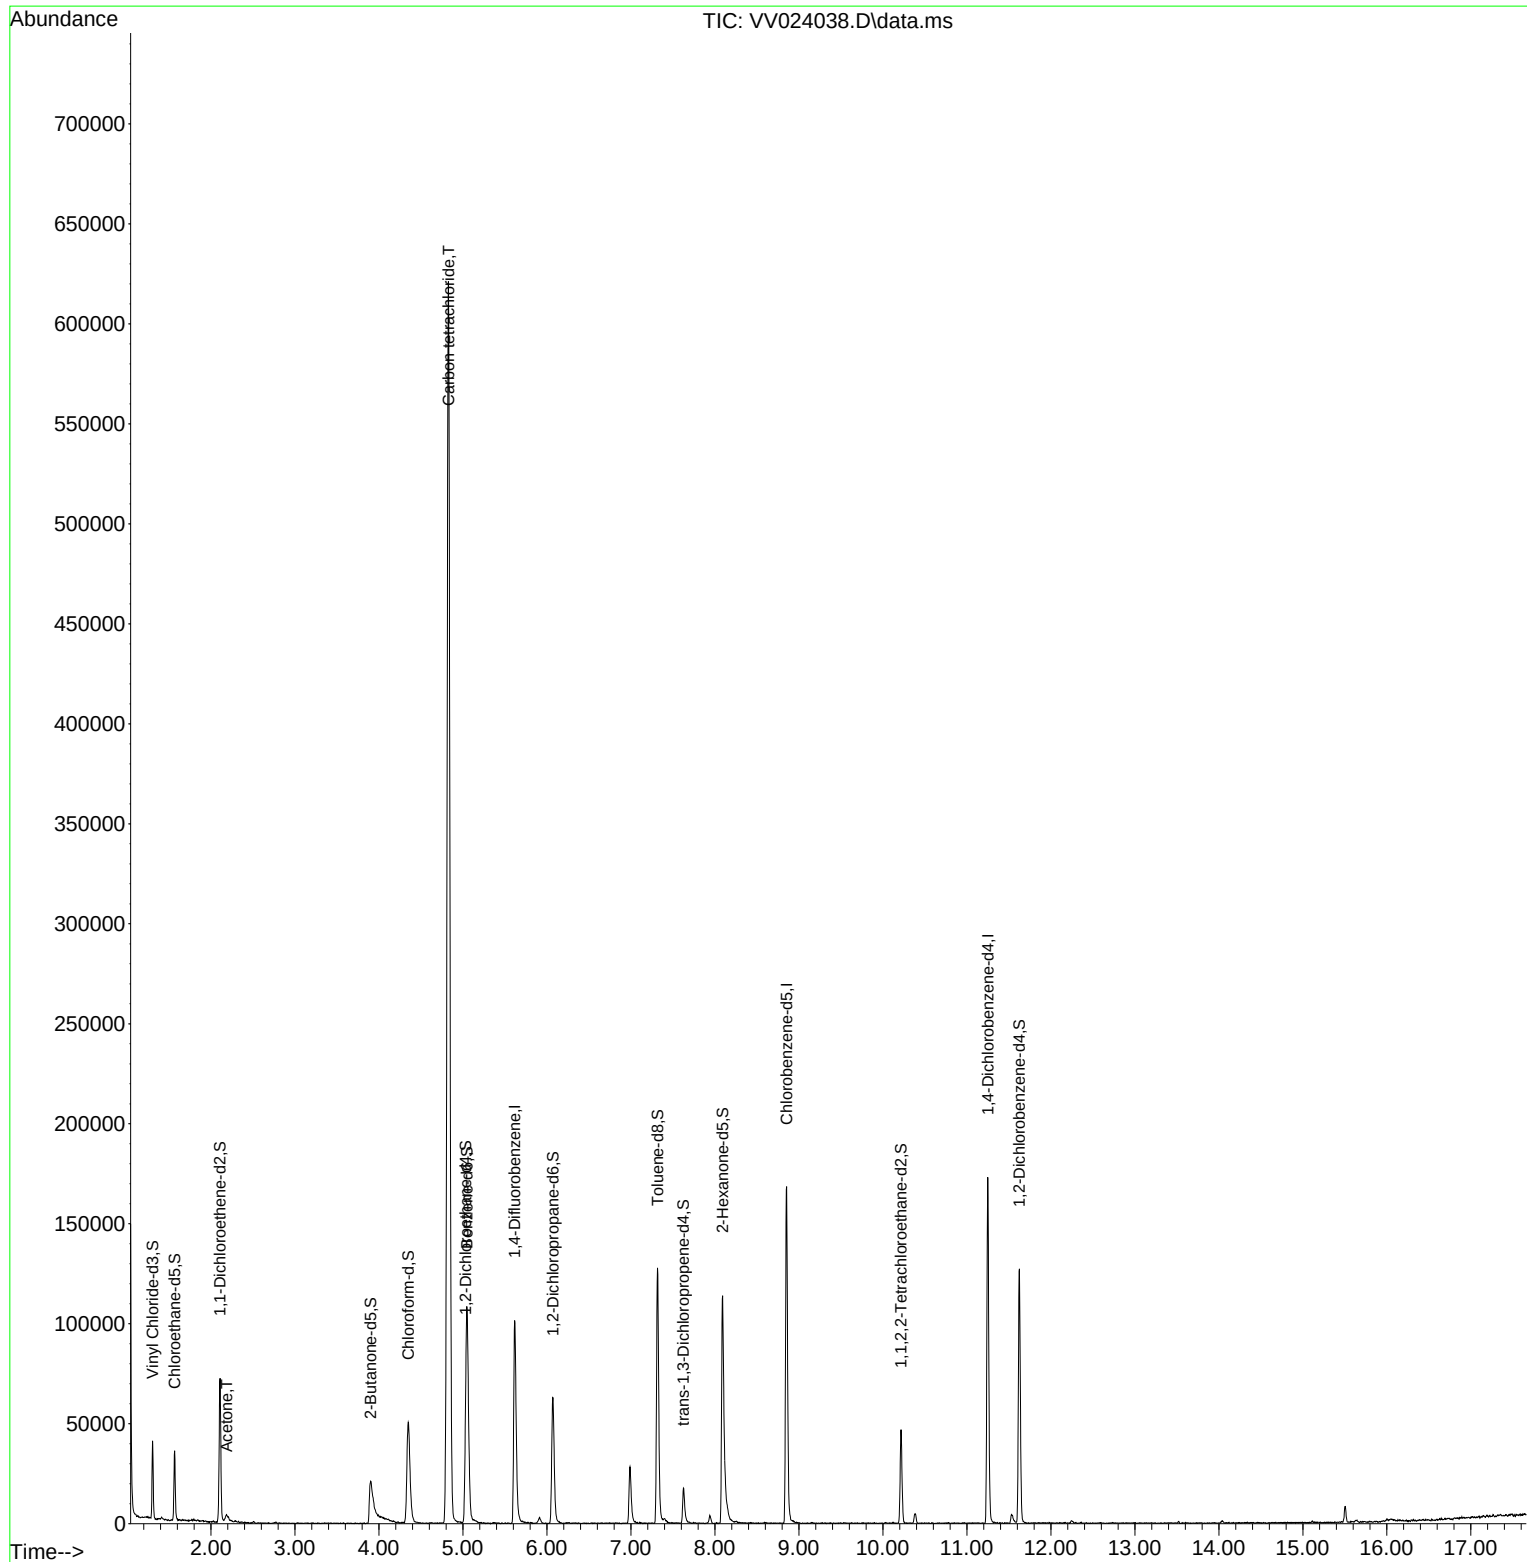


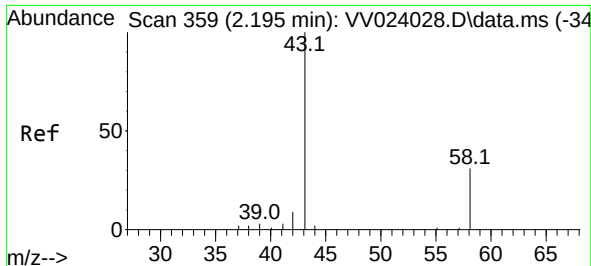

#13
Acetone
Concen: 8.414 ug/L
RT: 2.185 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV024038.D
Acq: 17 Dec 2021 02:06

Instrument :
MSVOA_V
ClientSampleId :
GBBJ1

Tgt Ion: 43 Resp: 6488
Ion Ratio Lower Upper
43 100
58 21.8 0.0 41.4

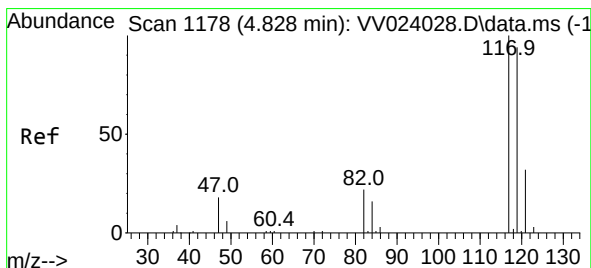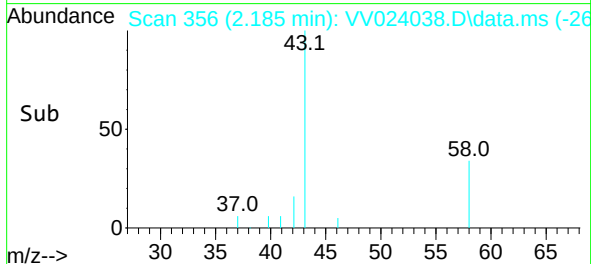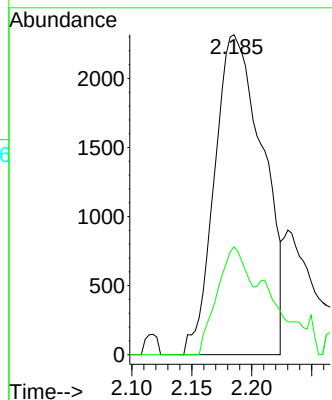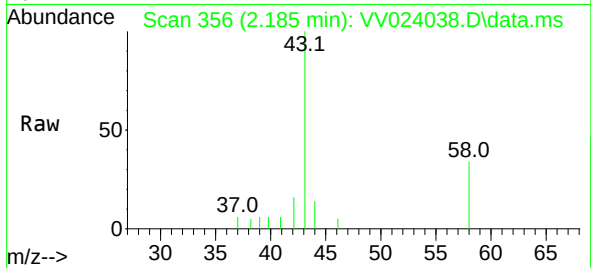

#31
Carbon tetrachloride
Concen: 36.566 ug/L
RT: 4.828 min Scan# 1178
Delta R.T. 0.003 min
Lab File: VV024038.D
Acq: 17 Dec 2021 02:06

Tgt Ion: 117 Resp: 447110
Ion Ratio Lower Upper
117 100
119 97.4 76.6 114.8

