

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024039.D
 Acq On : 17 Dec 2021 02:30
 Operator : SY/MD
 Sample : M5133-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ2

Quant Time: Dec 17 05:34:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	89632	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	94614	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47081	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23380	4.852	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.568	69	20920	5.204	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.000%
11) 1,1-Dichloroethene-d2	2.108	63	35886	3.815	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	3.905	46	40806	43.346	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.700%
24) Chloroform-d	4.352	84	54232	4.969	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.034	65	26977	5.309	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.050	84	99472	5.308	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
36) 1,2-Dichloropropane-d6	6.072	67	29335	5.189	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.800%
41) Toluene-d8	7.317	98	87329	5.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
43) trans-1,3-Dichloroprop...	7.625	79	10117	4.313	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.092	63	42435	40.415	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.820%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	20805	4.436	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	36391	5.787	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.800%
Target Compounds						Qvalue
13) Acetone	2.191	43	6525	8.664	ug/L	99
31) Carbon tetrachloride	4.828	117	180926	15.549	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024039.D
Acq On : 17 Dec 2021 02:30
Operator : SY/MD
Sample : M5133-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ2

Quant Time: Dec 17 05:34:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

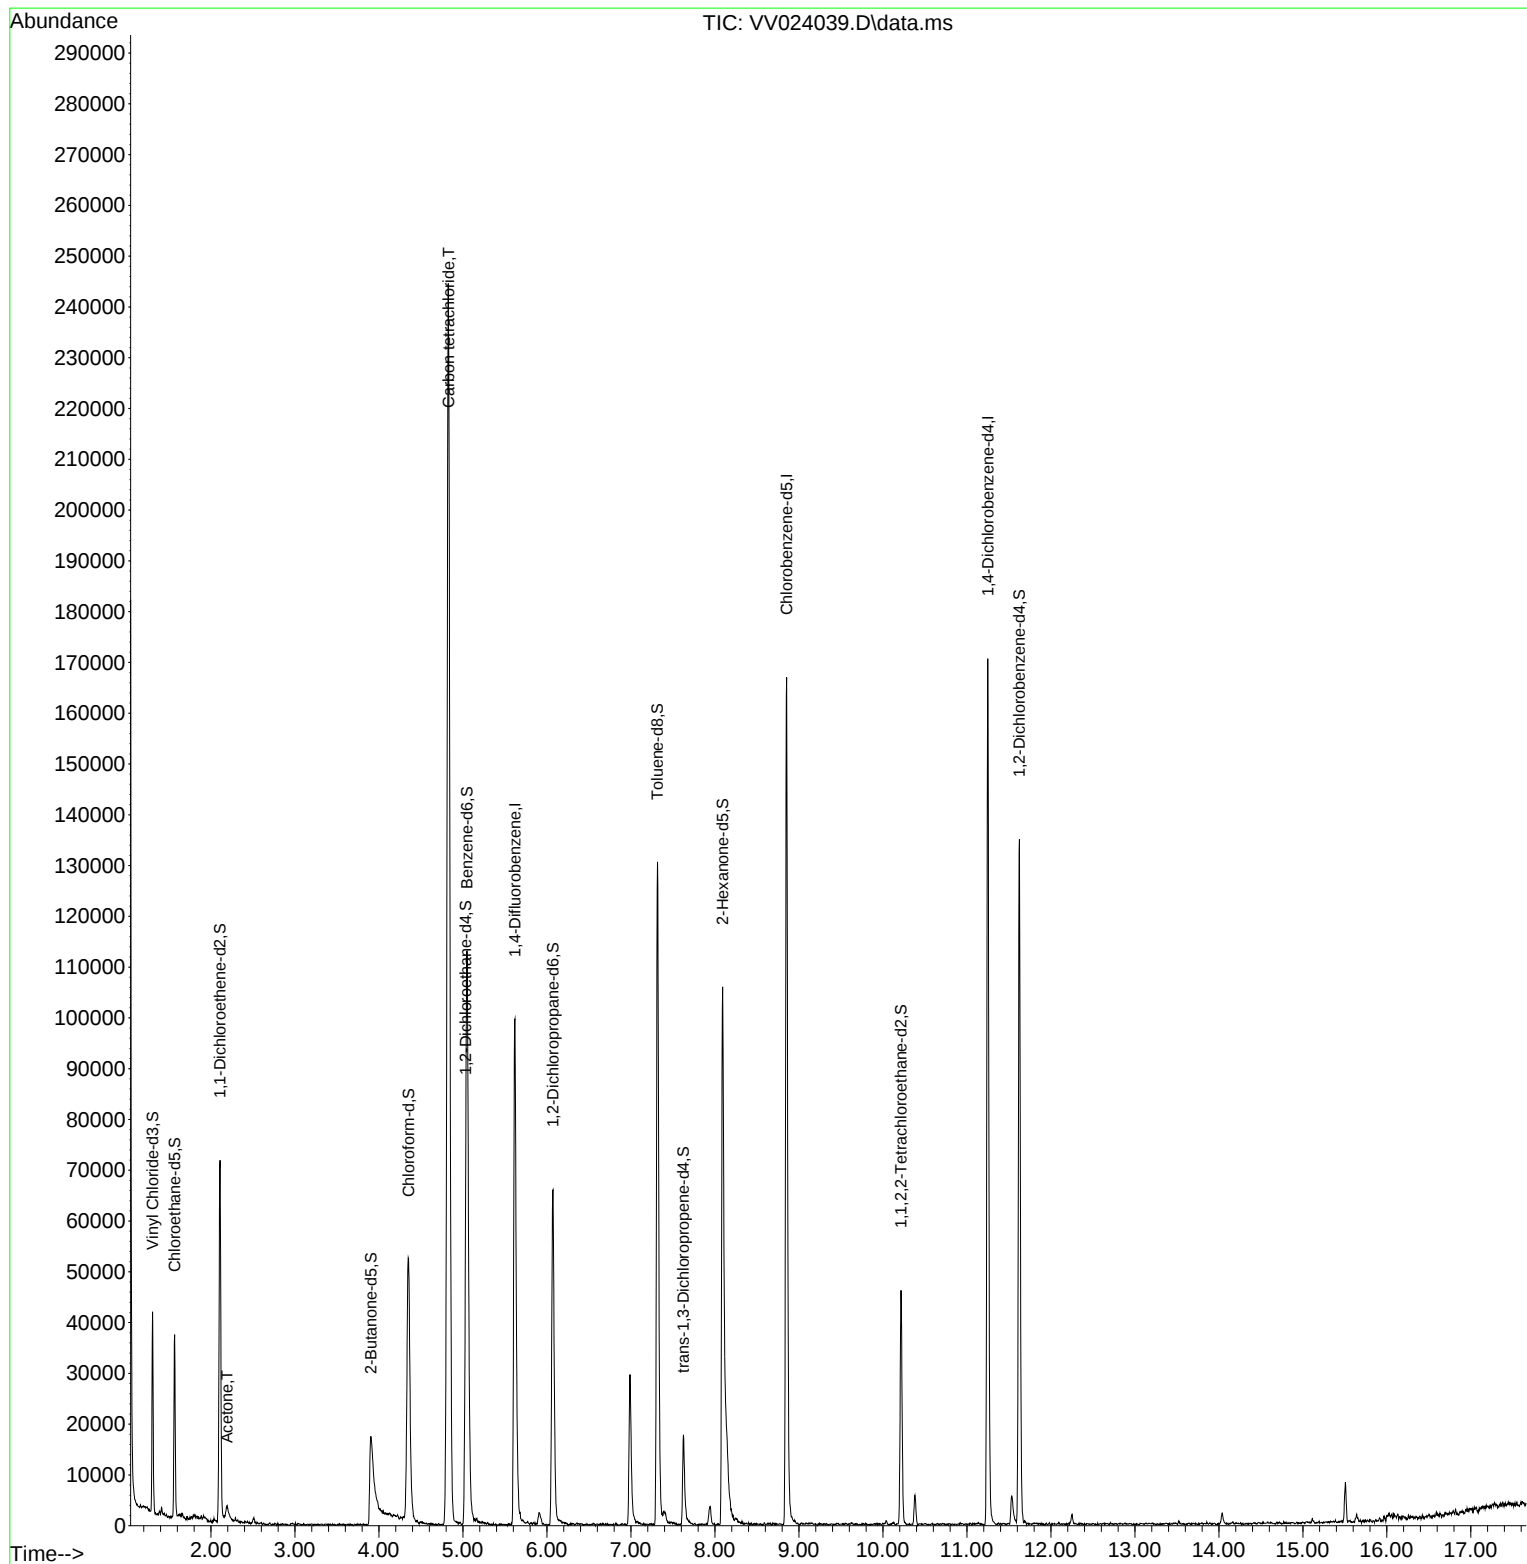

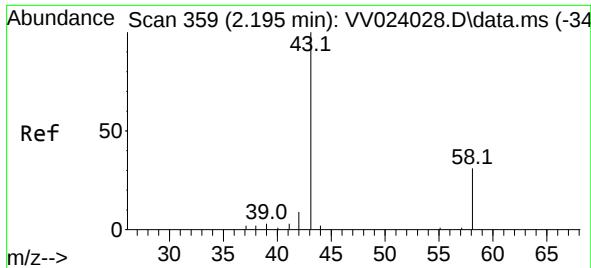

#13

Acetone

Concen: 8.664 ug/L

RT: 2.191 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV024039.D

Acq: 17 Dec 2021 02:30

Instrument :

MSVOA_V

ClientSampleId :





GBBJ2

Tgt Ion: 43 Resp: 6525

Ion Ratio Lower Upper

43 100

58 21.1 0.0 41.4

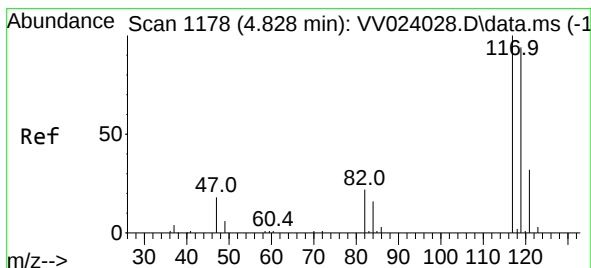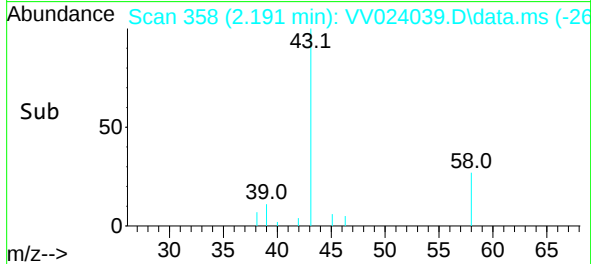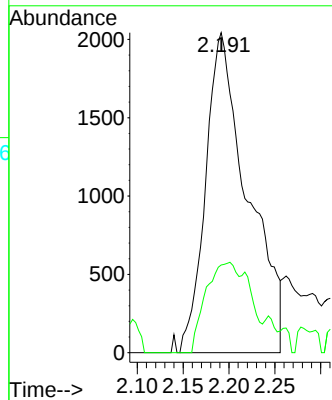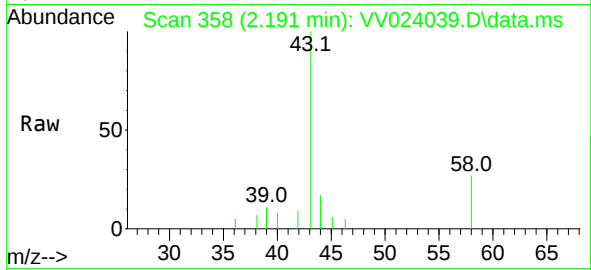

#31

Carbon tetrachloride

Concen: 15.549 ug/L

RT: 4.828 min Scan# 1178

Delta R.T. 0.003 min

Lab File: VV024039.D

Acq: 17 Dec 2021 02:30

Tgt Ion: 117 Resp: 180926

Ion Ratio Lower Upper

117 100

119 96.1 76.6 114.8

