

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
 Data File : VW024047.D
 Acq On : 17 Dec 2021 05:41
 Operator : SY/MD
 Sample : M5133-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBK0

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/17/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 07:44:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	92567	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	95562	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47160	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23707	4.764	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.200%	
7) Chloroethane-d5	1.568	69	21006	5.059	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.108	63	37292	3.839	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	76.800%	
20) 2-Butanone-d5	3.908	46	46050	47.366	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.740%	
24) Chloroform-d	4.349	84	55191	4.896	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	5.034	65	27872	5.311	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.200%	
32) Benzene-d6	5.050	84	104472	5.520	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.400%	
36) 1,2-Dichloropropane-d6	6.072	67	31047	5.437	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.800%	
41) Toluene-d8	7.317	98	91064	5.344	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.800%	
43) trans-1,3-Dichloroprop...	7.625	79	10419	4.398	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.000%	
46) 2-Hexanone-d5	8.092	63	42511	40.086	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.180%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21526	4.544	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	36948	5.865	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	117.400%	
Target Compounds					Qvalue	
13) Acetone	2.201	43	17637	22.675	ug/L	71
21) 2-Butanone	4.008	43	13444m	12.097	ug/L	
30) Cyclohexane	4.670	56	2203	0.222	ug/L #	21
31) Carbon tetrachloride	4.828	117	2023111	172.144	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024047.D
Acq On : 17 Dec 2021 05:41
Operator : SY/MD
Sample : M5133-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GBBK0

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/17/2021
Supervised By : Mahesh Dadoda 12/22/2021


Quant Time: Dec 17 07:44:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

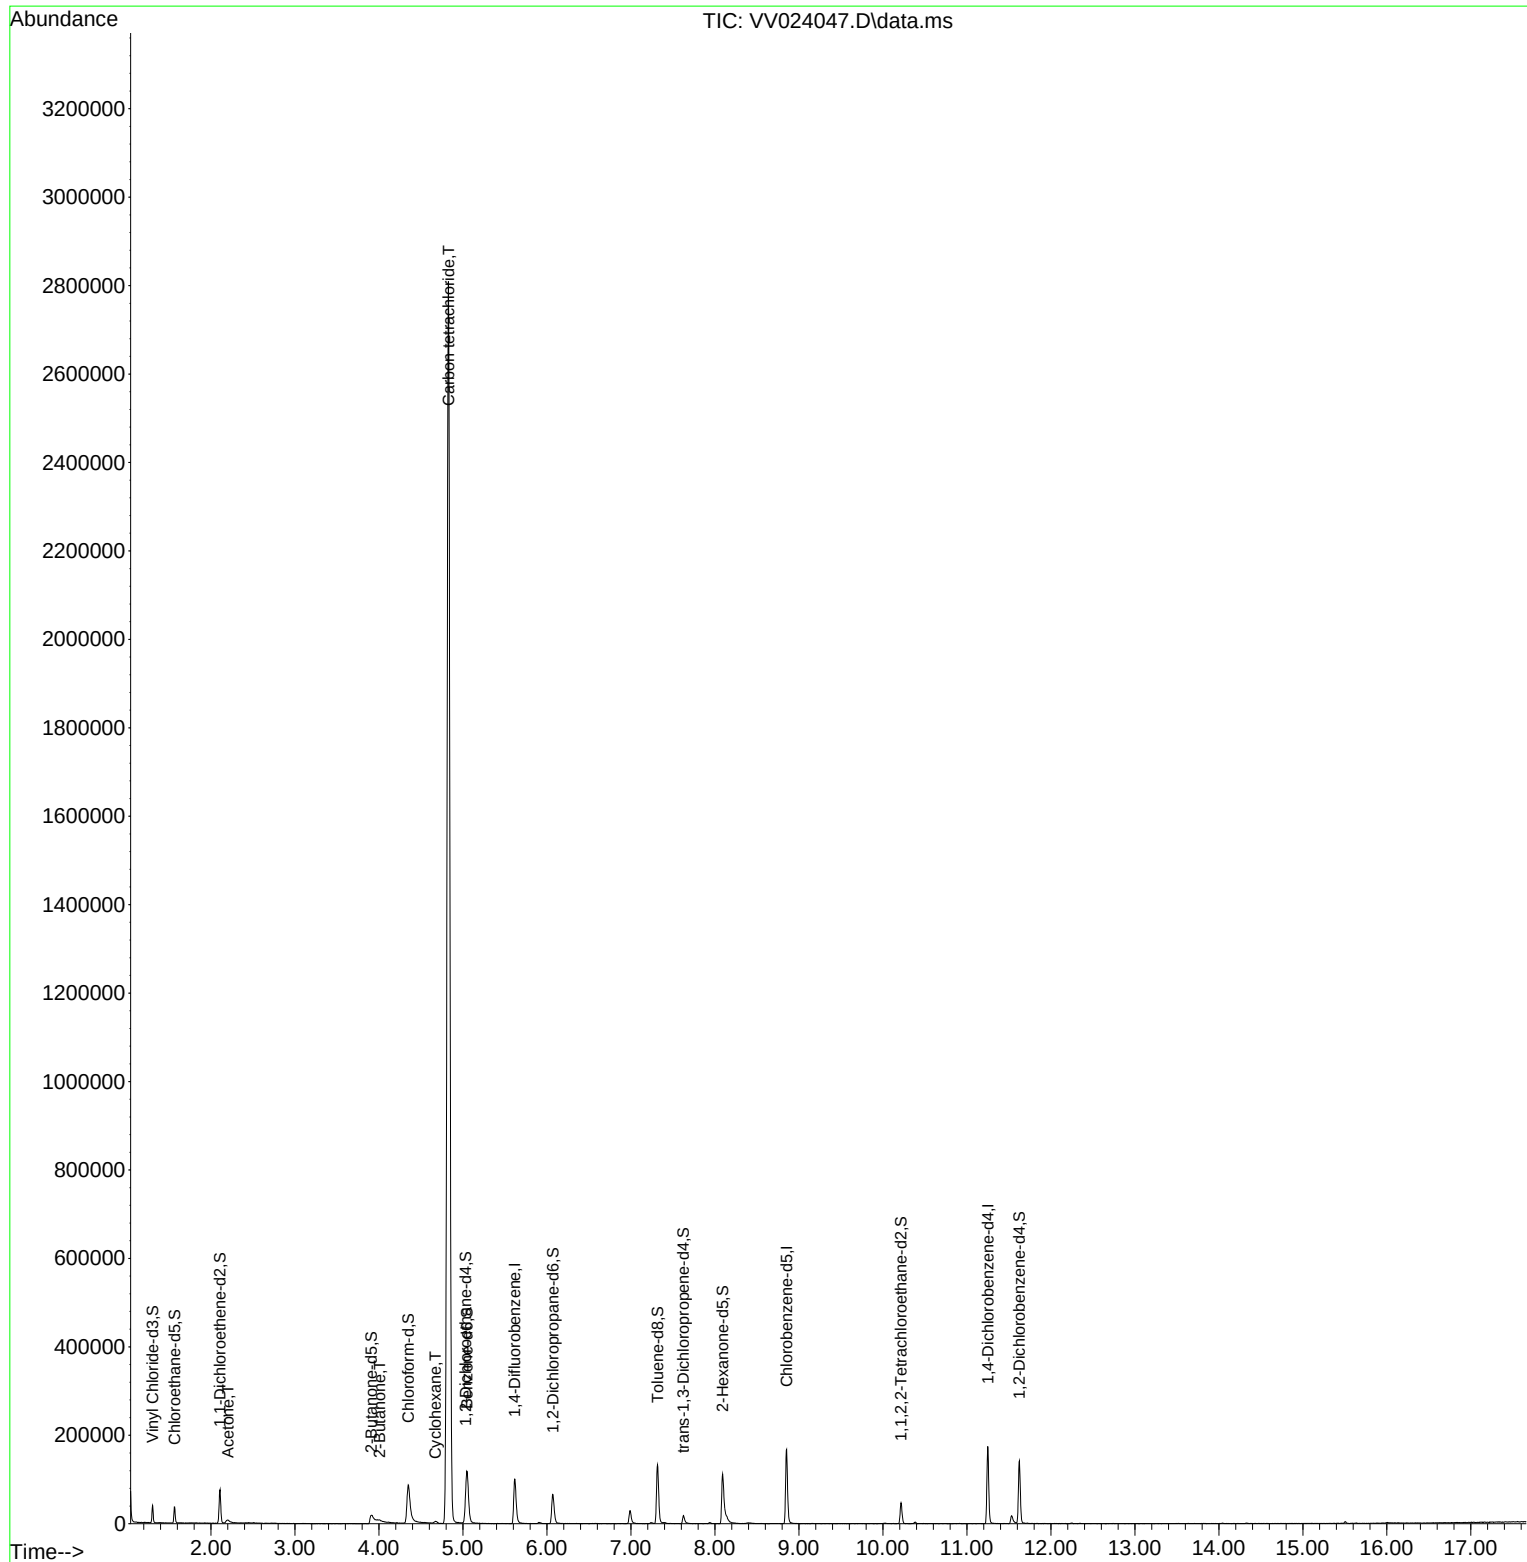

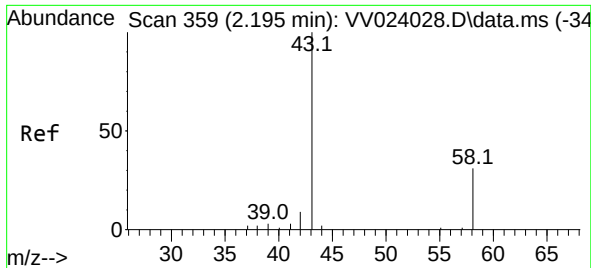

#13
Acetone
Concen: 22.675 ug/L
RT: 2.201 min Scan# 30
Delta R.T. 0.003 min
Lab File: VV024047.D
Acq: 17 Dec 2021 05:41




Instrument :
MSVOA_V
ClientSampleId :
GBBK0

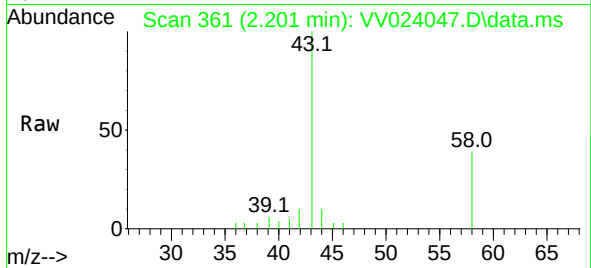

Tgt Ion: 43 Resp: 1763
Ion Ratio Lower Upper
43 100
58 34.2 0.0 41.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/22/2021

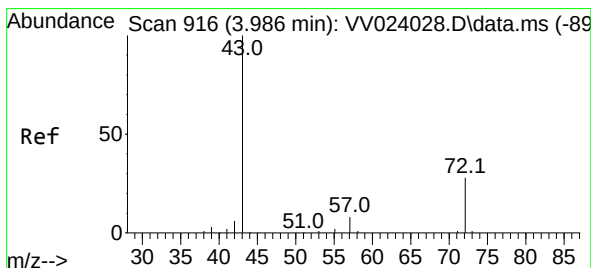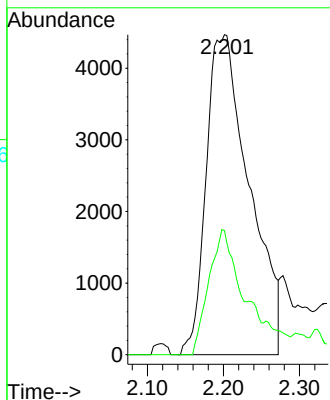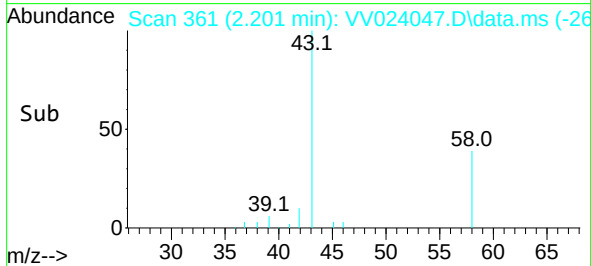

#21
2-Butanone
Concen: 12.097 ug/L m
RT: 4.008 min Scan# 923
Delta R.T. 0.019 min
Lab File: VV024047.D
Acq: 17 Dec 2021 05:41


Tgt Ion: 43 Resp: 13444
Ion Ratio Lower Upper
43 100
72 2.8 11.1 33.1#

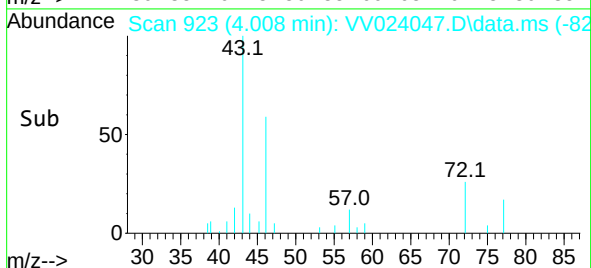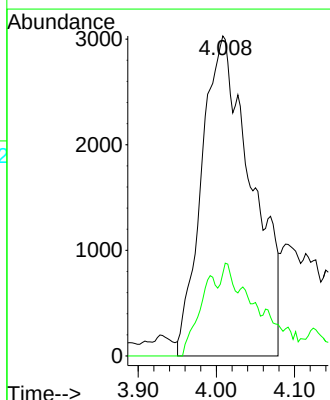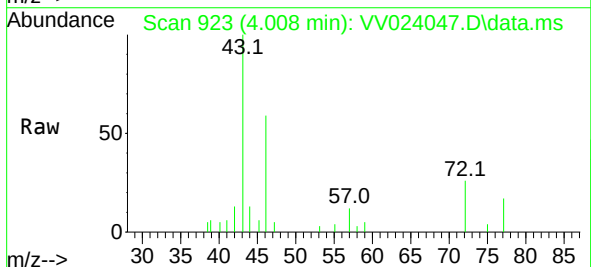

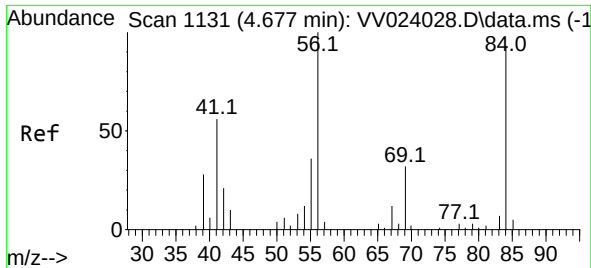

#30
Cyclohexane
Concen: 0.222 ug/L
RT: 4.670 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VV024047.D
Acq: 17 Dec 2021 05:41




Instrument :
MSVOA_V
ClientSampleId :
GBBK0

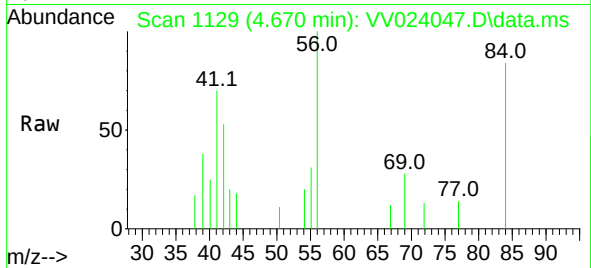

Tgt Ion: 56 Resp: 220
Ion Ratio Lower Upper
56 100
69 19.7 24.8 37.2
84 0.0 75.9 113.9

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/22/2021

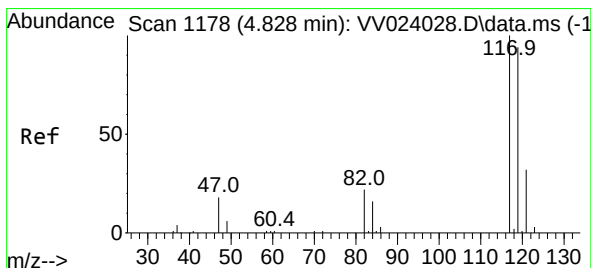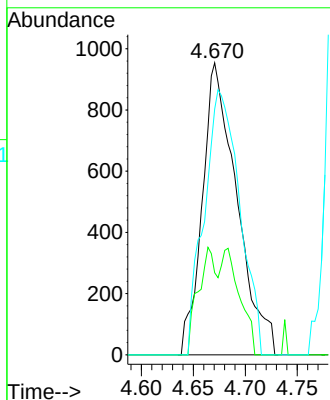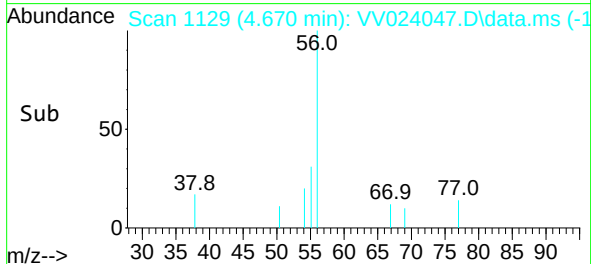

#31
Carbon tetrachloride
Concen: 172.144 ug/L
RT: 4.828 min Scan# 1178
Delta R.T. 0.003 min
Lab File: VV024047.D
Acq: 17 Dec 2021 05:41

Tgt Ion:117 Resp: 2023111
Ion Ratio Lower Upper
117 100
119 96.6 76.6 114.8

