

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
 Data File : VV024008.D
 Acq On : 16 Dec 2021 13:16
 Operator : SY/MD
 Sample : M5090-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3C2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	30	rVB3	3987	4232	1.44%	0.184%
2	1.307	75	83	96	rVB	25793	27962	9.52%	1.213%
3	1.417	110	117	124	rVB	4727	5988	2.04%	0.260%
4	1.568	157	164	173	rBV	27997	31177	10.62%	1.352%
5	2.108	321	332	344	rBV	44386	64783	22.06%	2.810%
6	2.770	525	538	553	rBV3	8107	17857	6.08%	0.774%
7	3.892	871	887	913	rBV2	41994	141752	48.28%	6.148%
8	4.349	1014	1029	1053	rBV2	47900	118363	40.31%	5.134%
9	5.047	1229	1246	1269	rBV3	87129	223477	76.11%	9.692%
10	5.619	1412	1424	1443	rBV	105918	215735	73.47%	9.357%
11	5.915	1507	1516	1530	rVB6	2001	4145	1.41%	0.180%
12	6.069	1552	1564	1586	rBV3	55757	117962	40.17%	5.116%
13	6.989	1841	1850	1868	rBV	24194	44580	15.18%	1.933%
14	7.317	1942	1952	1972	rBV	82005	145547	49.57%	6.313%
15	7.628	2040	2049	2068	rBV	14826	27043	9.21%	1.173%
16	8.088	2183	2192	2234	rBV	151602	290599	98.97%	12.604%
17	8.854	2419	2430	2453	rBV	178796	293627	100.00%	12.735%
18	10.217	2843	2854	2867	rBV	52234	80761	27.50%	3.503%
19	11.249	3165	3175	3191	rBV	175507	277283	94.43%	12.026%
20	11.625	3281	3292	3311	rBV	109924	172801	58.85%	7.495%




Sum of corrected areas: 2305674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024008.D
Acq On : 16 Dec 2021 13:16
Operator : SY/MD
Sample : M5090-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

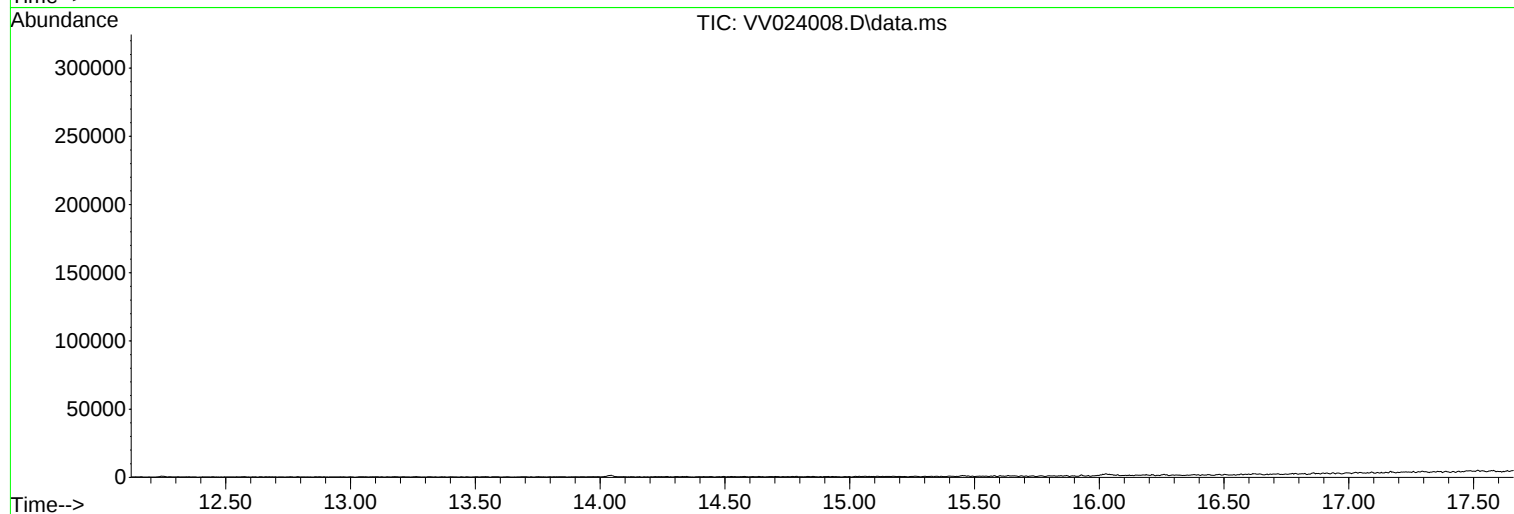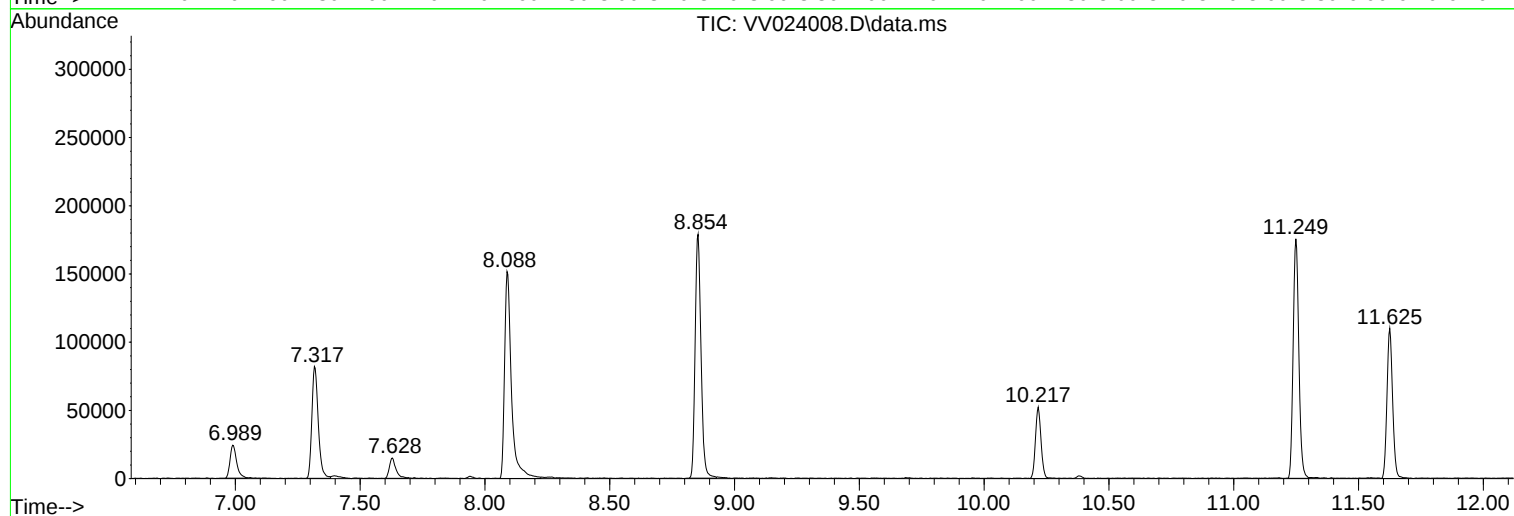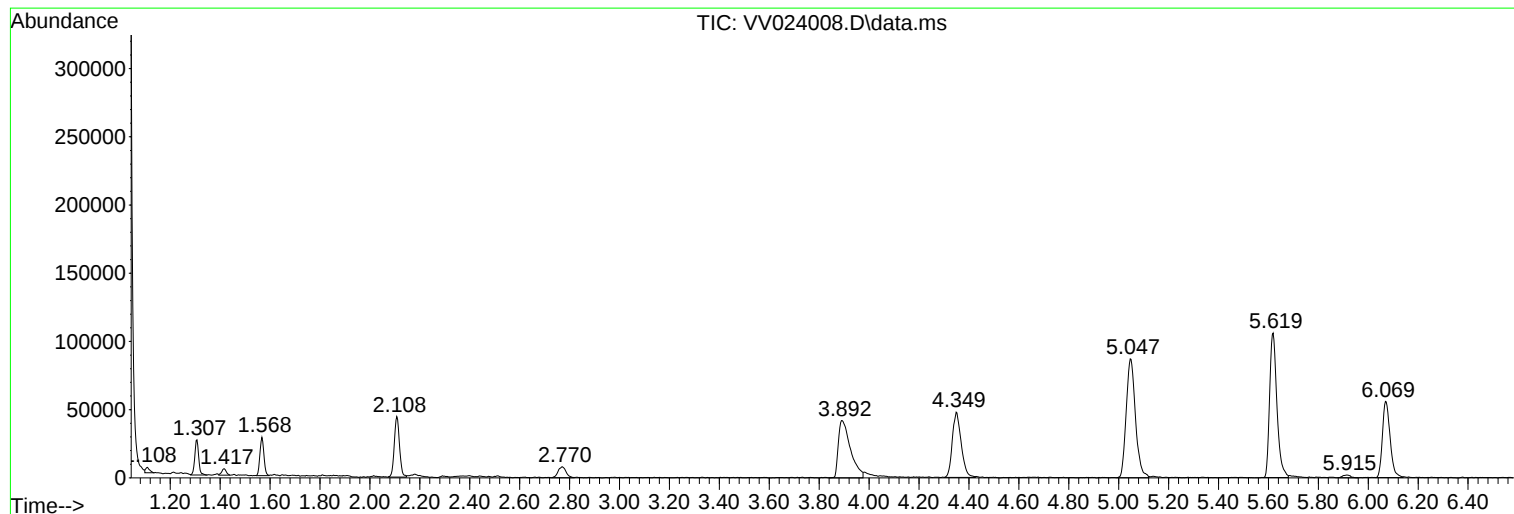

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024008.D
Acq On : 16 Dec 2021 13:16
Operator : SY/MD
Sample : M5090-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024008.D
Acq On : 16 Dec 2021 13:16
Operator : SY/MD
Sample : M5090-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
