

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
 Data File : VV024013.D
 Acq On : 16 Dec 2021 15:16
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK246

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	91	rVB	46047	45239	2.05%	0.938%
2	1.568	156	164	173	rBV	35863	41414	1.87%	0.859%
3	2.105	321	331	348	rVB	77501	110512	5.00%	2.293%
4	3.912	877	893	917	rBV3	59293	176831	8.00%	3.668%
5	4.349	1015	1029	1053	rVB2	51306	127515	5.77%	2.645%
6	5.047	1231	1246	1273	rBV2	113833	286765	12.97%	5.949%
7	5.619	1412	1424	1448	rBV2	107967	221251	10.01%	4.590%
8	6.069	1550	1564	1587	rBV2	63646	134297	6.08%	2.786%
9	6.989	1840	1850	1869	rBV2	31003	58786	2.66%	1.219%
10	7.317	1941	1952	1973	rBV	136989	240456	10.88%	4.988%
11	7.625	2039	2048	2069	rBV2	18427	33244	1.50%	0.690%
12	8.092	2182	2193	2228	rBV2	113424	245280	11.10%	5.088%
13	8.854	2419	2430	2452	rBV	180464	298440	13.50%	6.191%
14	10.217	2843	2854	2868	rBV	46330	73483	3.32%	1.524%
15	11.249	3164	3175	3191	rBV	193081	297879	13.48%	6.179%
16	11.625	3280	3292	3307	rBV	136584	218944	9.91%	4.542%
17	15.503	4486	4498	4518	rBV	1626340	2210192	100.00%	45.850%




Sum of corrected areas: 4820528

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024013.D
Acq On : 16 Dec 2021 15:16
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

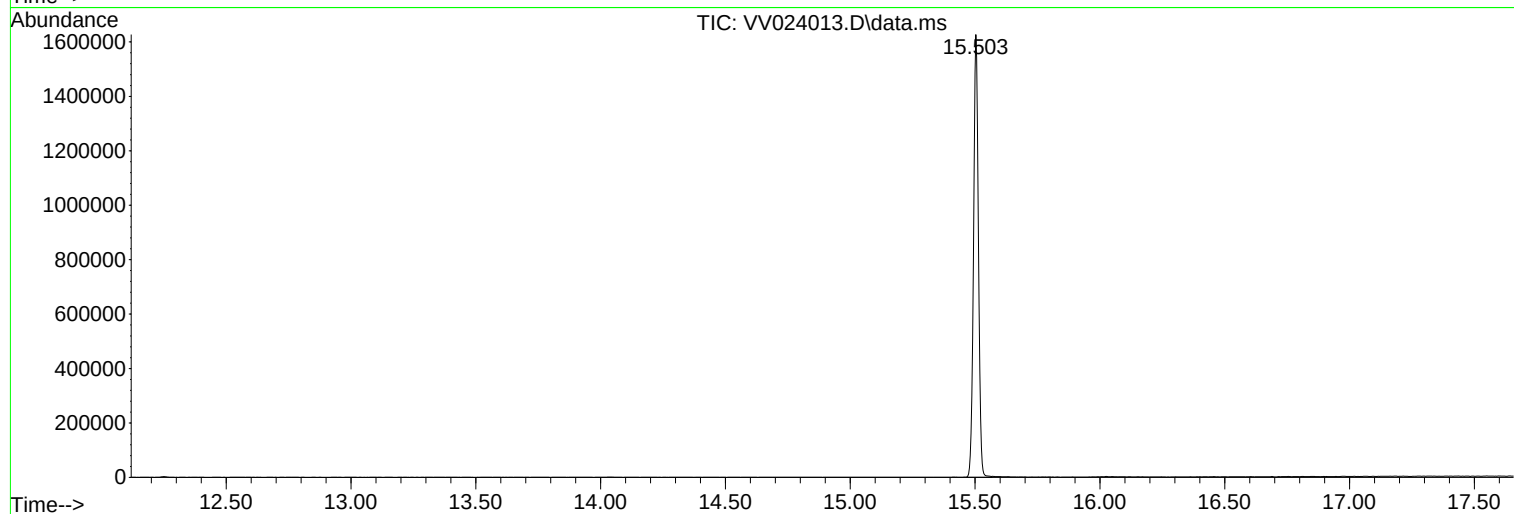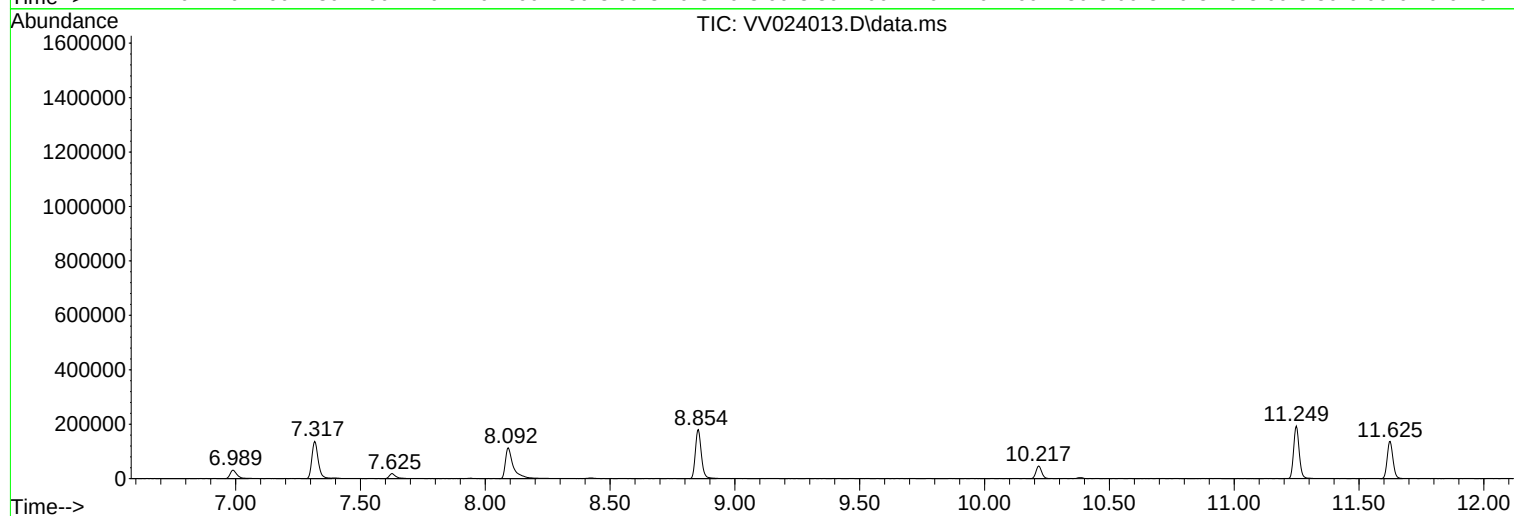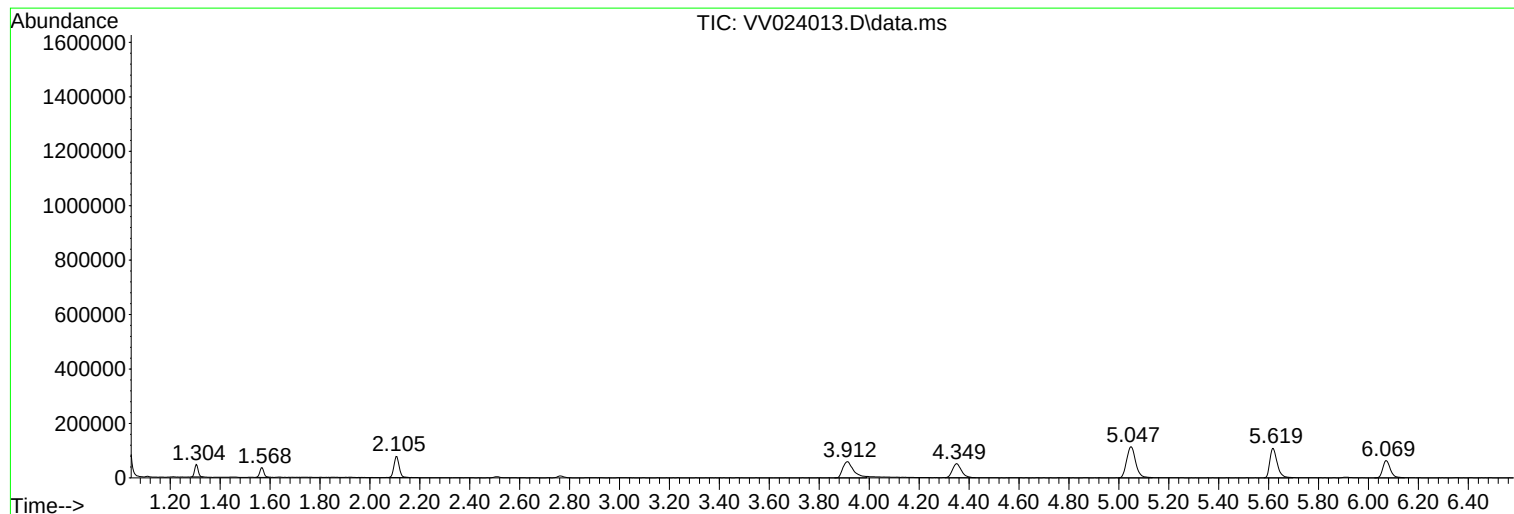

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024013.D
Acq On : 16 Dec 2021 15:16
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Diphenyl ether Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.503	37.10 ug/L	2210190	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diphenyl ether	170	C12H10O	000101-84-8	96
2			Diphenyl ether	170	C12H10O	000101-84-8	93
3			Diphenyl ether	170	C12H10O	000101-84-8	91
4			Diphenyl ether	170	C12H10O	000101-84-8	90
5			Spiro[cyclopropane-1,1'(4'H)-nap...	170	C12H10O	033498-24-7	81

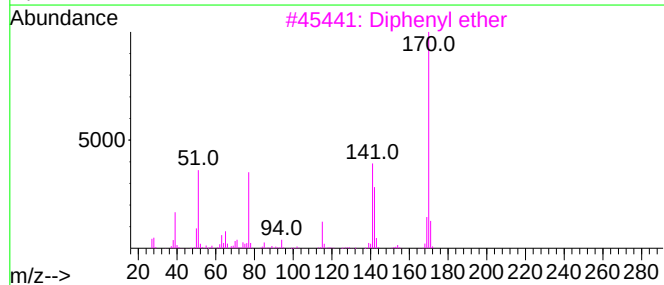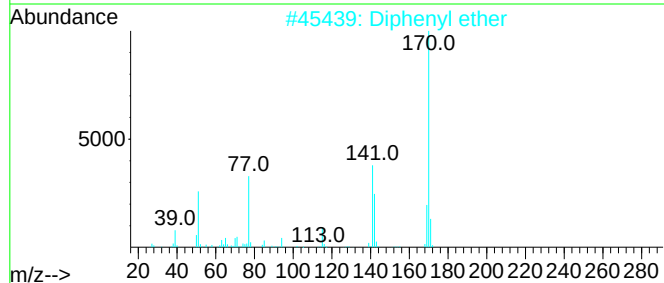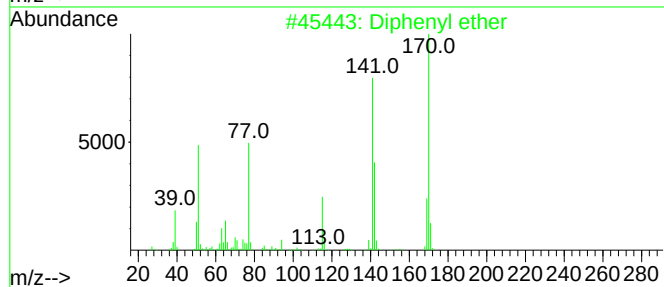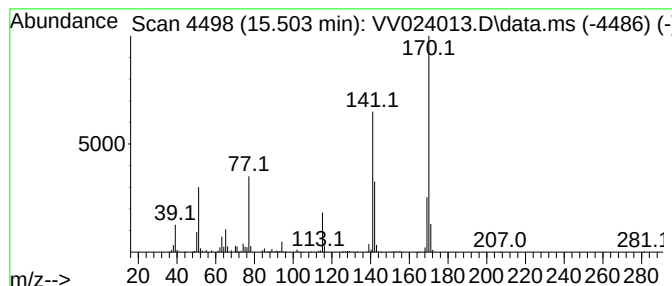

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121621\
Data File : VV024013.D
Acq On : 16 Dec 2021 15:16
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diphenyl ether	15.503	37.1	ug/L	2210190	3	11.249	297879	5.0