

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
 Data File : VV024045.D
 Acq On : 17 Dec 2021 04:53
 Operator : SY/MD
 Sample : M5133-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	91	rBV	40504	39988	5.36%	1.156%
2	1.568	154	164	175	rBV	35839	40763	5.46%	1.178%
3	2.105	322	331	346	rVB	68563	100080	13.41%	2.893%
4	2.195	346	359	374	rBV2	8047	25013	3.35%	0.723%
5	3.908	881	892	902	rBV2	19756	53317	7.14%	1.541%
6	3.979	904	914	944	rVB	47369	169659	22.73%	4.904%
7	4.349	1014	1029	1061	rBV3	86099	254934	34.15%	7.369%
8	4.828	1160	1178	1201	rBV	312890	746460	100.00%	21.577%
9	5.050	1230	1247	1275	rBV3	111925	278987	37.37%	8.064%
10	5.619	1412	1424	1452	rBV2	104540	215373	28.85%	6.225%
11	6.069	1552	1564	1580	rBV	63189	128959	17.28%	3.728%
12	6.989	1839	1850	1872	rBV2	28772	55131	7.39%	1.594%
13	7.317	1941	1952	1971	rBV	126456	224348	30.05%	6.485%
14	7.625	2035	2048	2068	rBV	17011	32315	4.33%	0.934%
15	8.092	2178	2193	2233	rBV3	105349	244102	32.70%	7.056%
16	8.854	2417	2430	2454	rBV	174641	283973	38.04%	8.208%
17	10.217	2844	2854	2865	rBV	44201	69433	9.30%	2.007%
18	10.381	2896	2905	2917	rVB2	5053	8078	1.08%	0.233%
19	11.249	3164	3175	3193	rBV	174674	269718	36.13%	7.796%
20	11.532	3255	3263	3279	rBV7	5766	12255	1.64%	0.354%
21	11.622	3281	3291	3310	rVB	128588	206694	27.69%	5.975%




Sum of corrected areas: 3459580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024045.D
Acq On : 17 Dec 2021 04:53
Operator : SY/MD
Sample : M5133-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

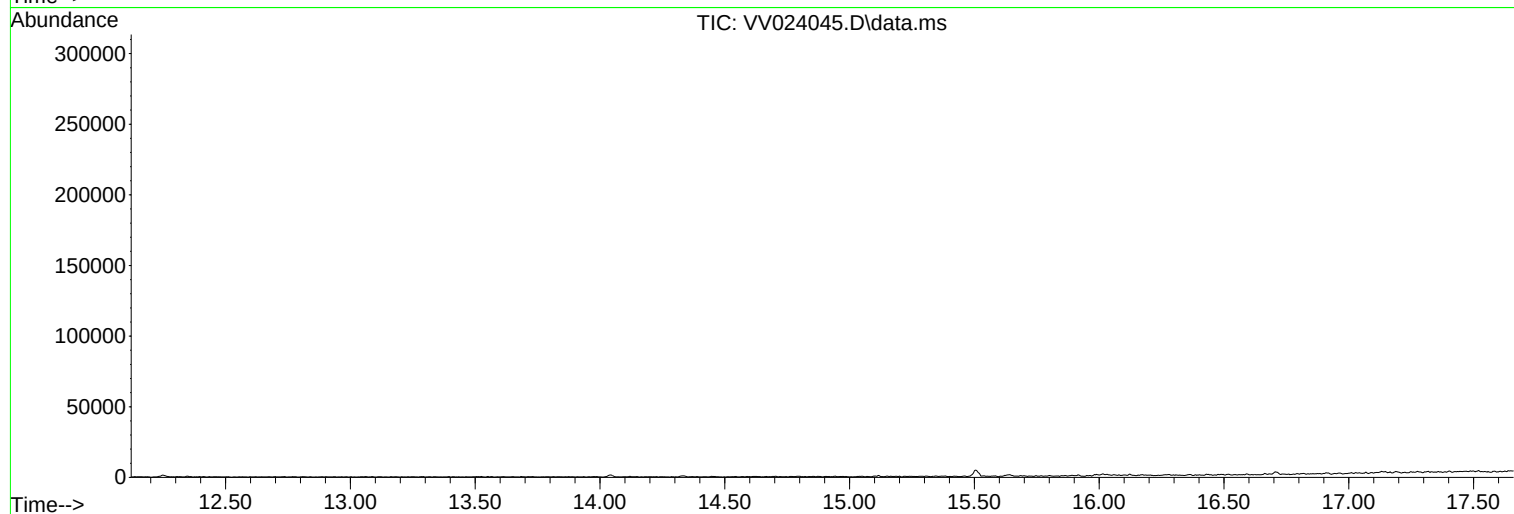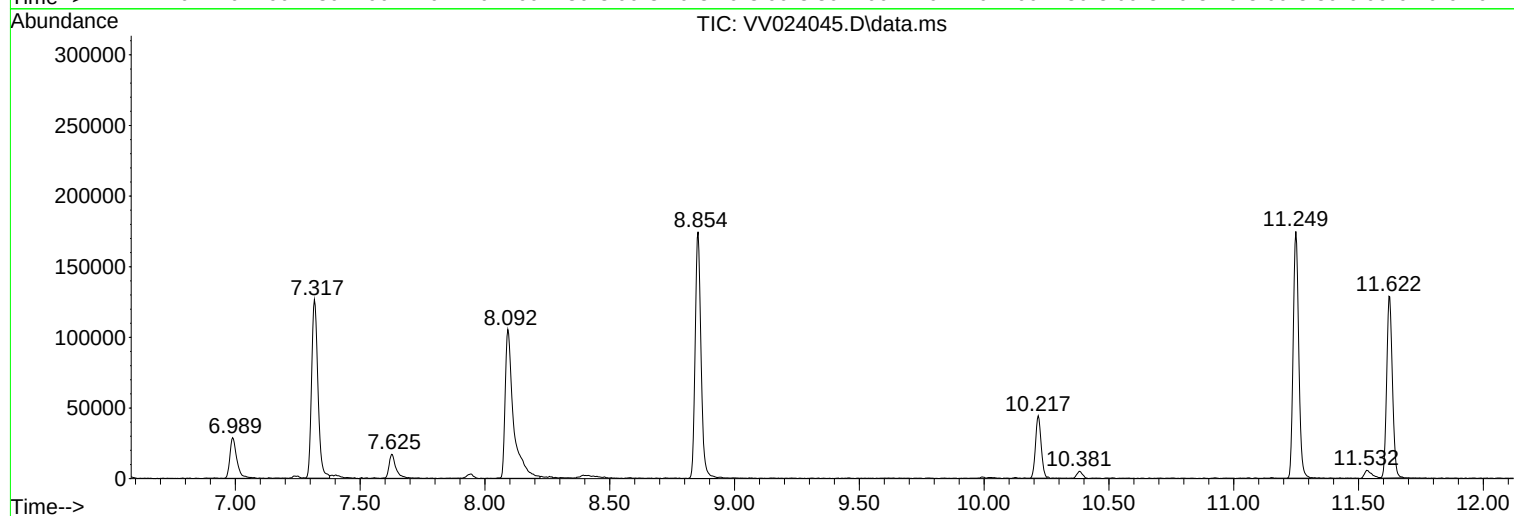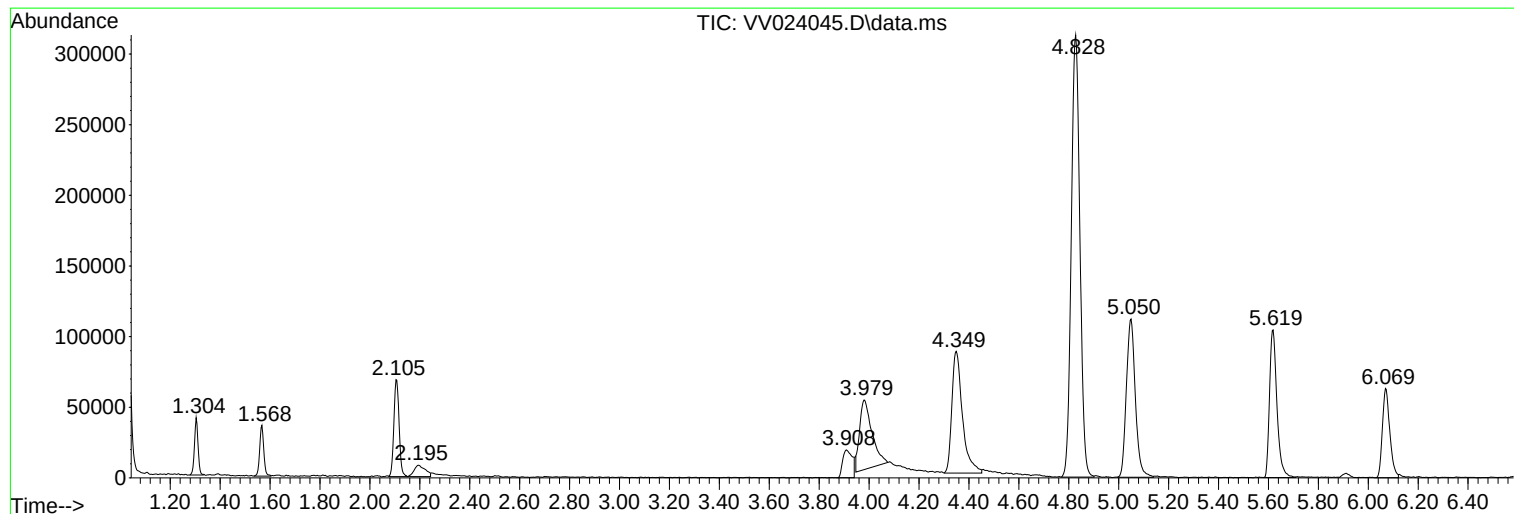

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024045.D
Acq On : 17 Dec 2021 04:53
Operator : SY/MD
Sample : M5133-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.989	1.28 ug/L	55131	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	.	.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	43	
2	Thiophosgene		114	CCl2S	000463-71-8	40	
3	Methane, oxybis[chloro-		114	C2H4Cl2O	000542-88-1	37	
4	1,3-Cyclohexadiene		80	C6H8	000592-57-4	32	
5	1,3,5-Hexatriene		80	C6H8	002235-12-3	32	

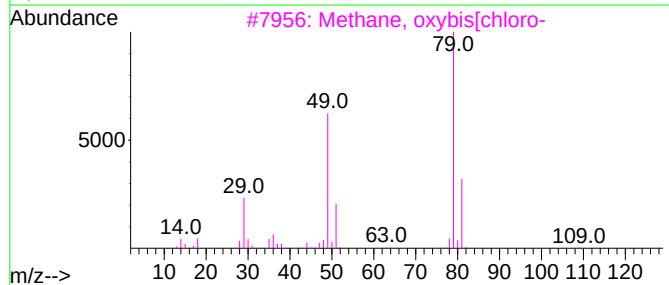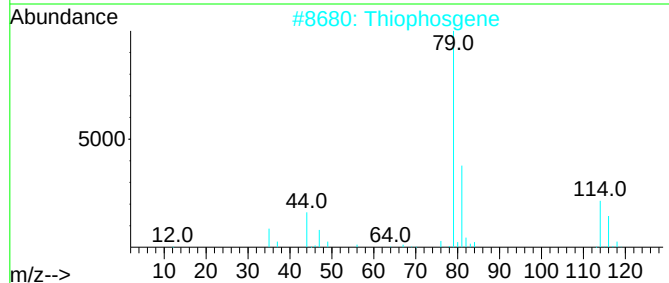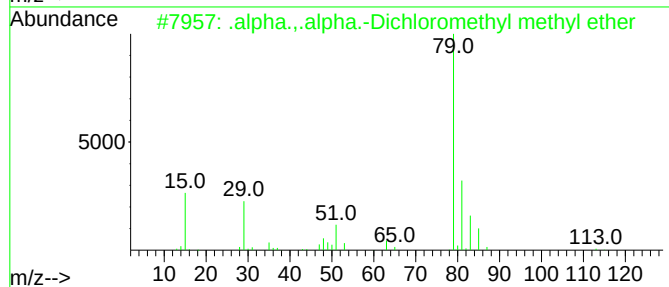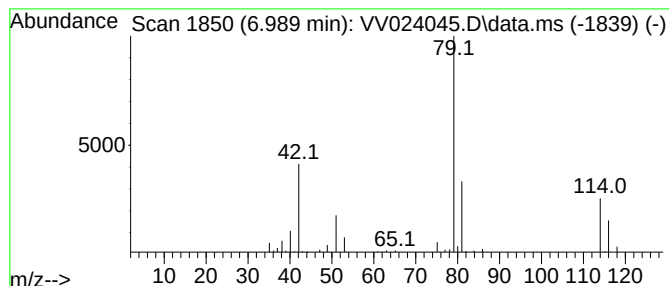

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV024045.D
Acq On : 17 Dec 2021 04:53
Operator : SY/MD
Sample : M5133-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.989	1.3	ug/L	55131	1	5.619	215373	5.0