
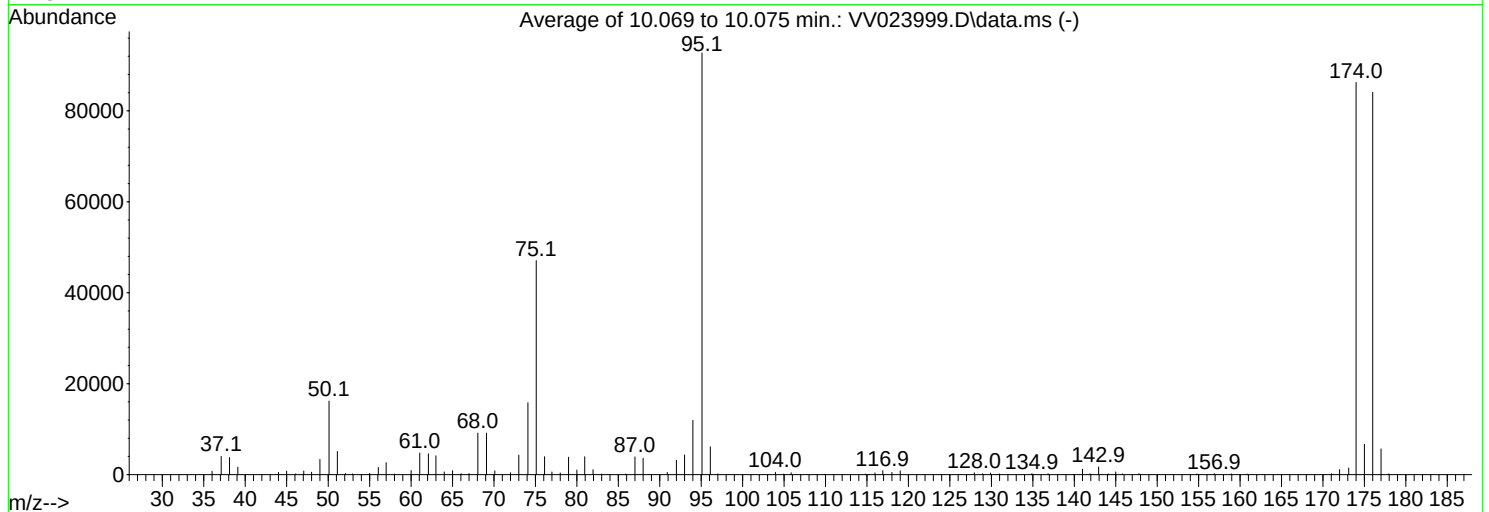


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121621\
Data File : VV023999.D
Acq On : 16 Dec 2021 09:27
Operator : SY/MD
Sample : BFB253
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB253

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Dec 20 04:04:22 2021

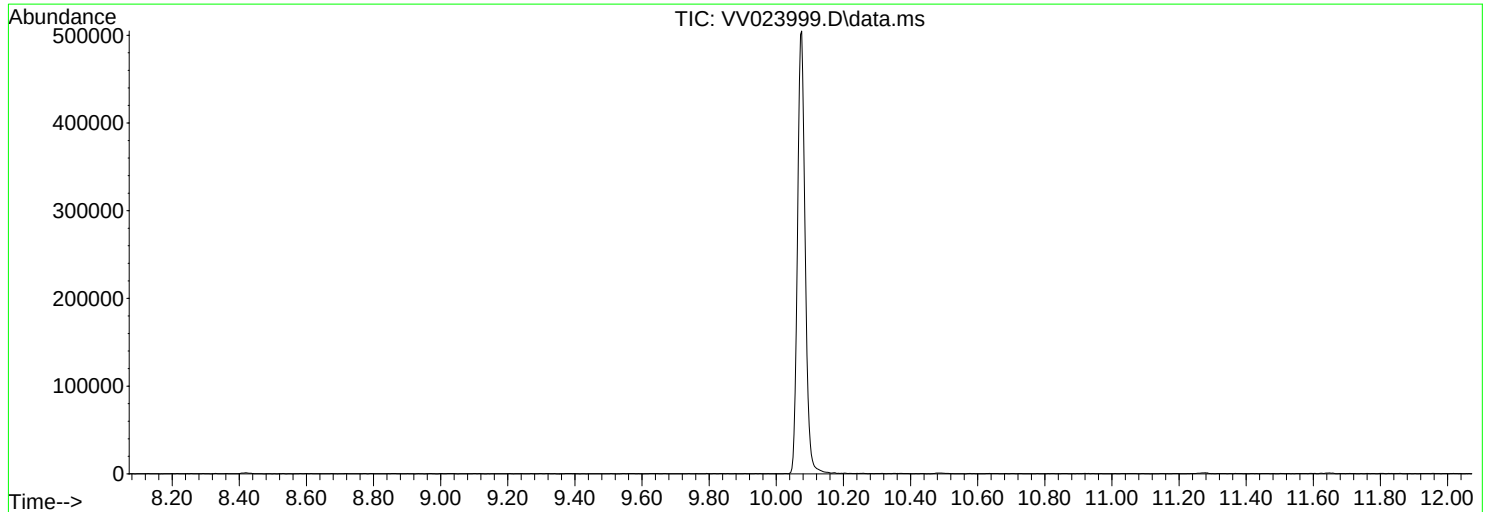

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	16176	PASS
75	95	30	80	50.7	47067	PASS
95	95	100	100	100.0	92755	PASS
96	95	5	9	6.6	6123	PASS
173	174	0.00	2	1.7	1489	PASS
174	95	50	120	93.0	86235	PASS
175	174	5	9	7.8	6692	PASS
176	174	95	105	97.5	84088	PASS
177	176	5	10	6.7	5652	PASS

m/z	Abundance
39.90	144.0
44.00	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	695.0
37.10	3845.0
38.10	3596.0
39.10	1652.0
40.10	131.0
44.00	636.0
45.00	712.0
46.10	190.0
47.00	854.0
48.00	518.0
49.00	3174.0
50.10	15388.0
51.10	4941.0
52.00	276.0
52.90	169.0
55.10	287.0
56.10	1552.0
57.00	2456.0
58.00	142.0
60.00	845.0
61.00	4460.0
62.10	4382.0
63.00	3995.0
64.00	626.0
65.00	829.0
66.10	196.0
67.00	196.0
68.00	8785.0
69.10	8737.0
70.10	809.0
72.00	451.0
73.00	3957.0
74.10	14883.0
75.10	43672.0
76.10	3848.0
77.00	573.0
78.00	407.0
79.00	3441.0
80.00	987.0
80.90	3639.0
81.90	959.0
83.00	142.0
85.80	104.0
87.00	3656.0
88.00	3231.0
90.90	417.0
92.00	2918.0
93.00	3992.0
94.00	11066.0
95.10	87016.0
96.10	5678.0
97.00	153.0
103.90	504.0
105.00	101.0
105.90	357.0
114.80	114.0
115.20	129.0
116.00	333.0
116.90	817.0
118.00	445.0
119.00	796.0
124.00	107.0
127.90	390.0
129.00	211.0
129.90	331.0
130.90	170.0
134.90	256.0
136.80	202.0
141.00	1023.0
141.90	187.0
143.00	1627.0
144.10	126.0
145.00	528.0
145.80	186.0
147.80	179.0
154.80	280.0
156.90	232.0
158.90	185.0
160.80	128.0
171.10	225.0
172.00	1030.0
173.00	1371.0
174.00	77432.0
175.00	5924.0
176.00	75848.0
177.00	5171.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	780.0
37.10	4122.0
38.10	3905.0
39.10	1748.0
40.10	125.0
44.00	700.0
45.00	794.0
46.10	194.0
47.00	821.0
48.00	534.0
49.00	3420.0
50.10	16760.0
51.10	5330.0
52.10	267.0
53.00	186.0
55.00	287.0
56.10	1672.0
57.00	2751.0
58.00	147.0
60.00	948.0
61.00	4994.0
62.10	4667.0
63.00	4331.0
64.00	637.0
65.00	931.0
66.00	207.0
67.00	266.0
68.00	9541.0
69.10	9362.0
70.10	875.0
72.00	414.0
73.00	4454.0
74.10	16400.0
75.10	48496.0
76.10	4099.0
77.00	604.0
78.00	384.0
79.00	3980.0
80.00	1044.0
81.00	4062.0
81.90	1099.0
83.00	148.0
85.90	169.0
87.00	4077.0
88.00	3721.0
90.90	517.0
92.00	3238.0
93.00	4549.0
94.00	12316.0
95.10	96192.0
96.10	6346.0
97.00	167.0
103.90	524.0
104.90	154.0
105.80	417.0
107.00	107.0
109.90	119.0
114.80	142.0
115.90	387.0
116.90	935.0
118.00	523.0
119.00	864.0
123.90	109.0
128.00	439.0
128.90	220.0
129.90	373.0
131.00	204.0
134.90	251.0
136.80	227.0
139.90	130.0
141.00	1259.0
141.90	245.0
142.90	1763.0
144.10	174.0
145.00	643.0
145.80	192.0
147.80	237.0
154.80	264.0
156.90	270.0
158.90	180.0
160.90	151.0
171.00	242.0
172.00	1166.0
173.10	1545.0
174.00	88904.0
175.00	6969.0
176.00	86744.0
177.00	5796.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	743.0
37.10	4097.0
38.10	3821.0
39.10	1606.0
40.00	122.0
44.00	624.0
45.00	833.0
46.10	157.0
47.10	756.0
48.00	506.0
49.00	3451.0
50.10	16379.0
51.10	5075.0
52.20	254.0
53.00	181.0
54.90	275.0
56.00	1520.0
57.00	2734.0
58.00	135.0
60.00	979.0
61.10	4860.0
62.10	4641.0
63.00	4083.0
64.00	593.0
65.00	902.0
66.00	199.0
67.00	301.0
68.10	9082.0
69.10	9326.0
70.10	821.0
72.00	394.0
73.00	4508.0
74.10	16214.0
75.10	49032.0
76.10	3871.0
77.00	594.0
78.00	353.0
79.00	4068.0
80.00	1026.0
81.00	4126.0
82.00	1181.0
83.00	117.0
85.90	195.0
87.00	3980.0
88.00	3902.0
90.90	534.0
92.00	3300.0
93.00	4483.0
94.00	12353.0
95.10	95056.0
96.10	6345.0
97.00	198.0
104.00	499.0
104.90	185.0
105.80	469.0
106.90	125.0
109.90	118.0
110.90	124.0
114.80	156.0
115.90	400.0
116.90	892.0
118.00	527.0
119.00	863.0
128.00	398.0
128.90	210.0
129.90	388.0
131.00	193.0
134.90	219.0
136.90	227.0
139.90	138.0
141.00	1328.0
141.90	226.0
142.90	1724.0
144.10	180.0
145.00	683.0
145.80	201.0
147.80	283.0
155.00	251.0
156.90	292.0
159.00	170.0
160.90	147.0
171.00	207.0
172.00	1182.0
173.20	1552.0
174.00	92368.0
175.00	7183.0
176.00	89672.0
177.00	5989.0
177.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253