

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
 Data File : VV029693.D
 Acq On : 16 Dec 2022 12:46
 Operator : SY/MD
 Sample : VV1216WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Quant Time: Dec 16 20:18:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 16 20:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	248868	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	222451	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	109480	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	57631	3.763	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.200%
7) Chloroethane-d5	1.565	69	54467	4.858	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.102	63	79802	3.256	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.200%
20) 2-Butanone-d5	3.902	46	124460	48.578	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.160%
24) Chloroform-d	4.339	84	130755	4.783	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.024	65	59815	4.973	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.040	84	273842	4.454	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.060	67	84976	4.919	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.307	98	235953	4.066	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	7.616	79	25802	3.874	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.400%
46) 2-Hexanone-d5	8.085	63	128502	54.125	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.240%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	62379	5.852	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	117.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	88830	4.645	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	20012	1.024	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029693.D
Acq On : 16 Dec 2022 12:46
Operator : SY/MD
Sample : VV1216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287


Quant Time: Dec 16 20:18:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 16 20:17:28 2022
Response via : Initial Calibration

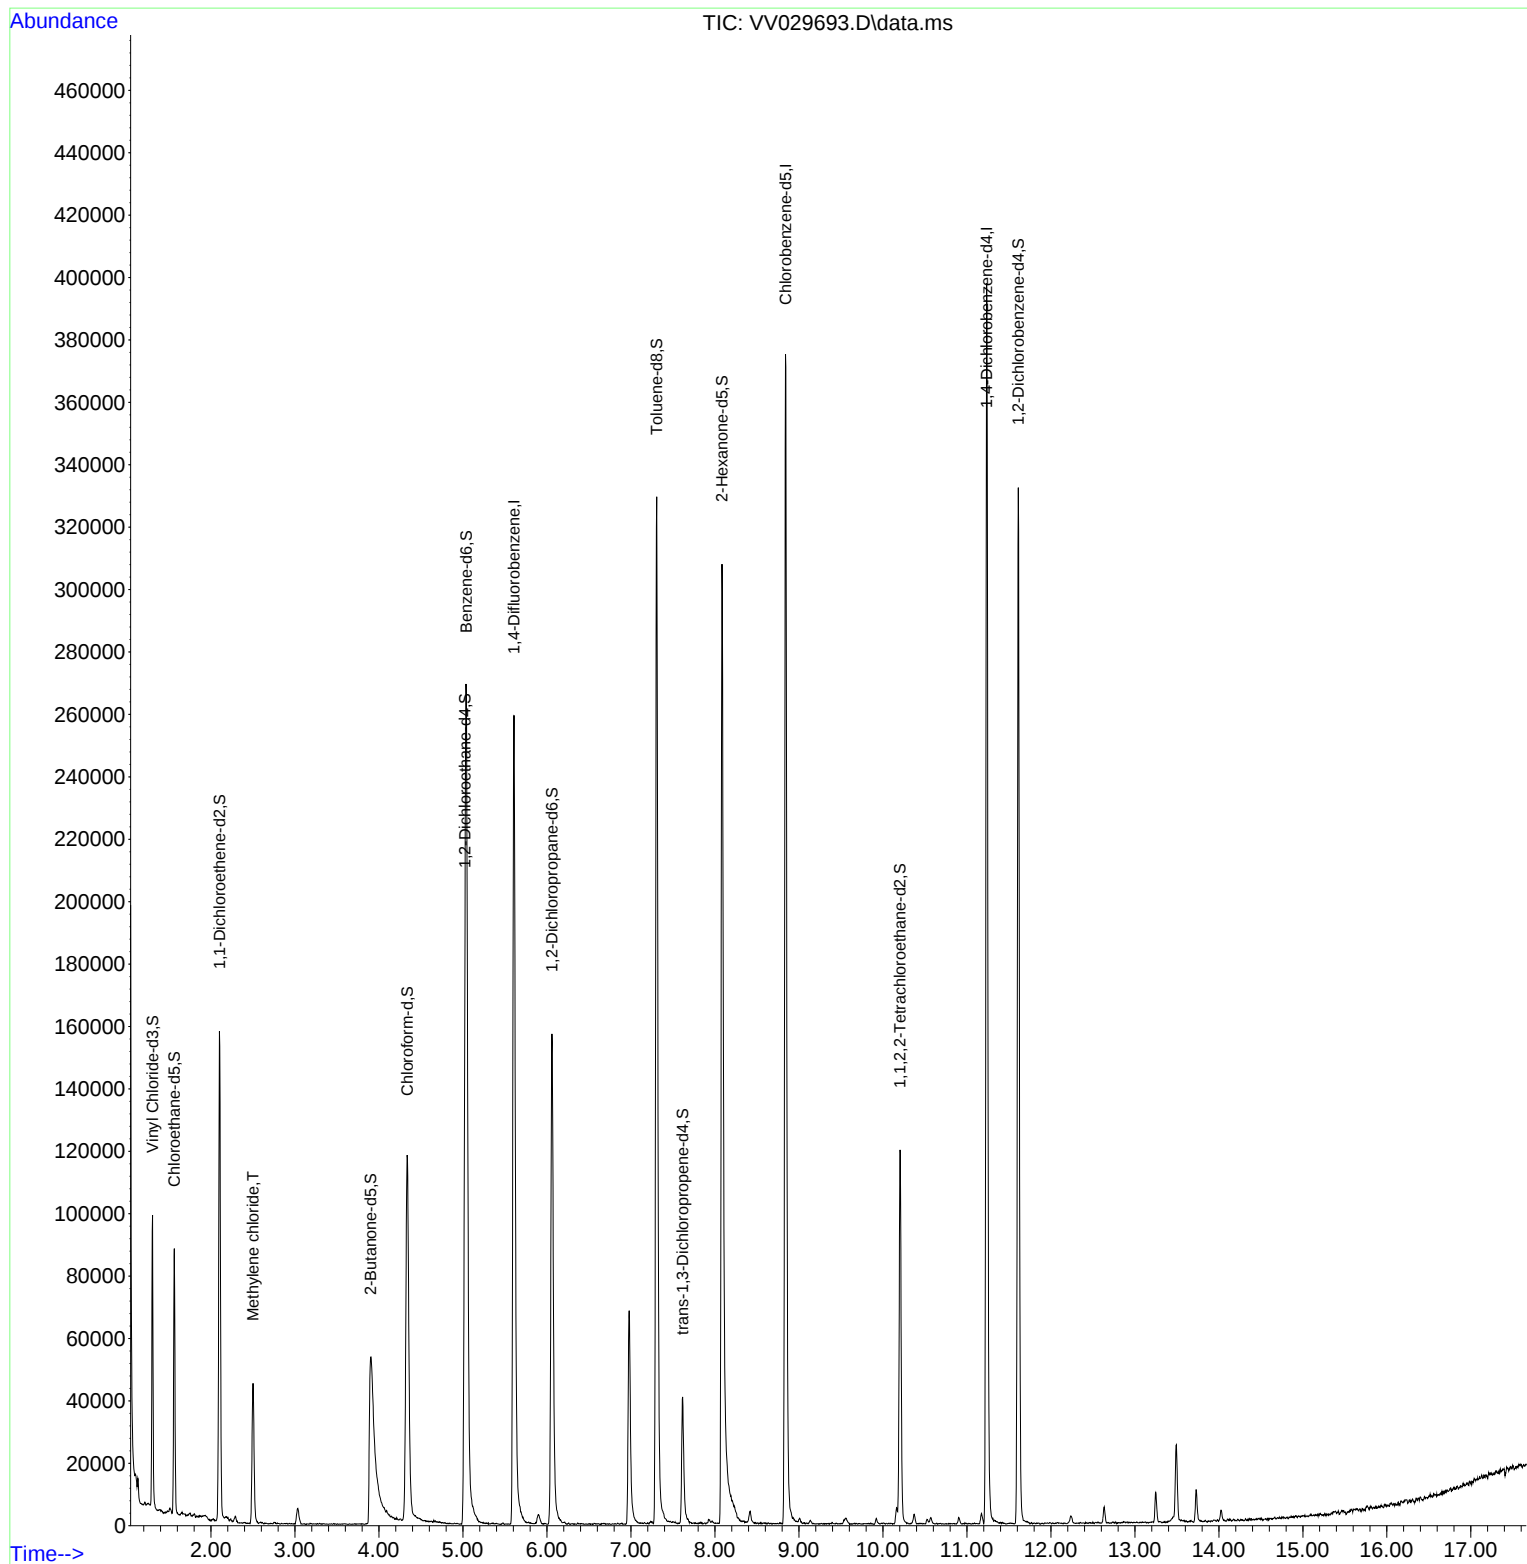

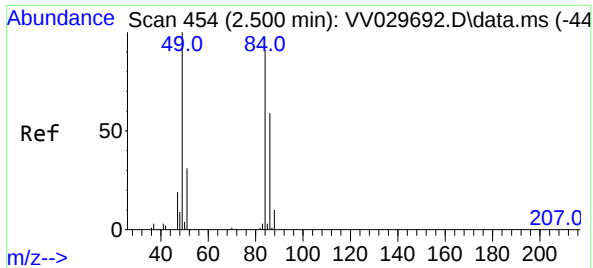

#16
Methylene chloride
Concen: 1.024 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV029693.D
Acq: 16 Dec 2022 12:46

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

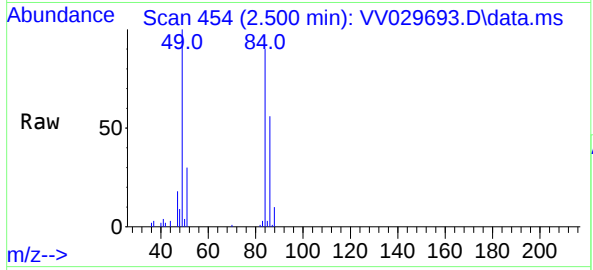

Tgt Ion: 84 Resp: 20012

Ion	Ratio	Lower	Upper
84	100		
86	61.9	45.6	84.6
49	111.3	77.8	144.4

