

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121622\
 Data File : VW029702.D
 Acq On : 16 Dec 2022 16:58
 Operator : SY/MD
 Sample : N6034-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGPL4

Quant Time: Dec 16 20:20:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 16 20:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	238657	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	222183	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	112860	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	46371	3.157	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.200%
7) Chloroethane-d5	1.565	69	46641	4.338	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.800%
11) 1,1-Dichloroethene-d2	2.105	63	68017	2.894	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.800%#
20) 2-Butanone-d5	3.899	46	139252	56.677	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.360%
24) Chloroform-d	4.339	84	114785	4.379	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.027	65	54100	4.690	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
32) Benzene-d6	5.044	84	231695	3.773	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.400%
36) 1,2-Dichloropropane-d6	6.063	67	73680	4.270	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.400%
41) Toluene-d8	7.310	98	196910	3.397	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	7.616	79	23294	3.502	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.085	63	124501	52.503	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.000%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	56476	5.304	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	82741	4.197	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.000%
Target Compounds					Qvalue	
13) Acetone	2.192	43	35302	19.761	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029702.D
Acq On : 16 Dec 2022 16:58
Operator : SY/MD
Sample : N6034-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPL4

Quant Time: Dec 16 20:20:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 16 20:17:28 2022
Response via : Initial Calibration

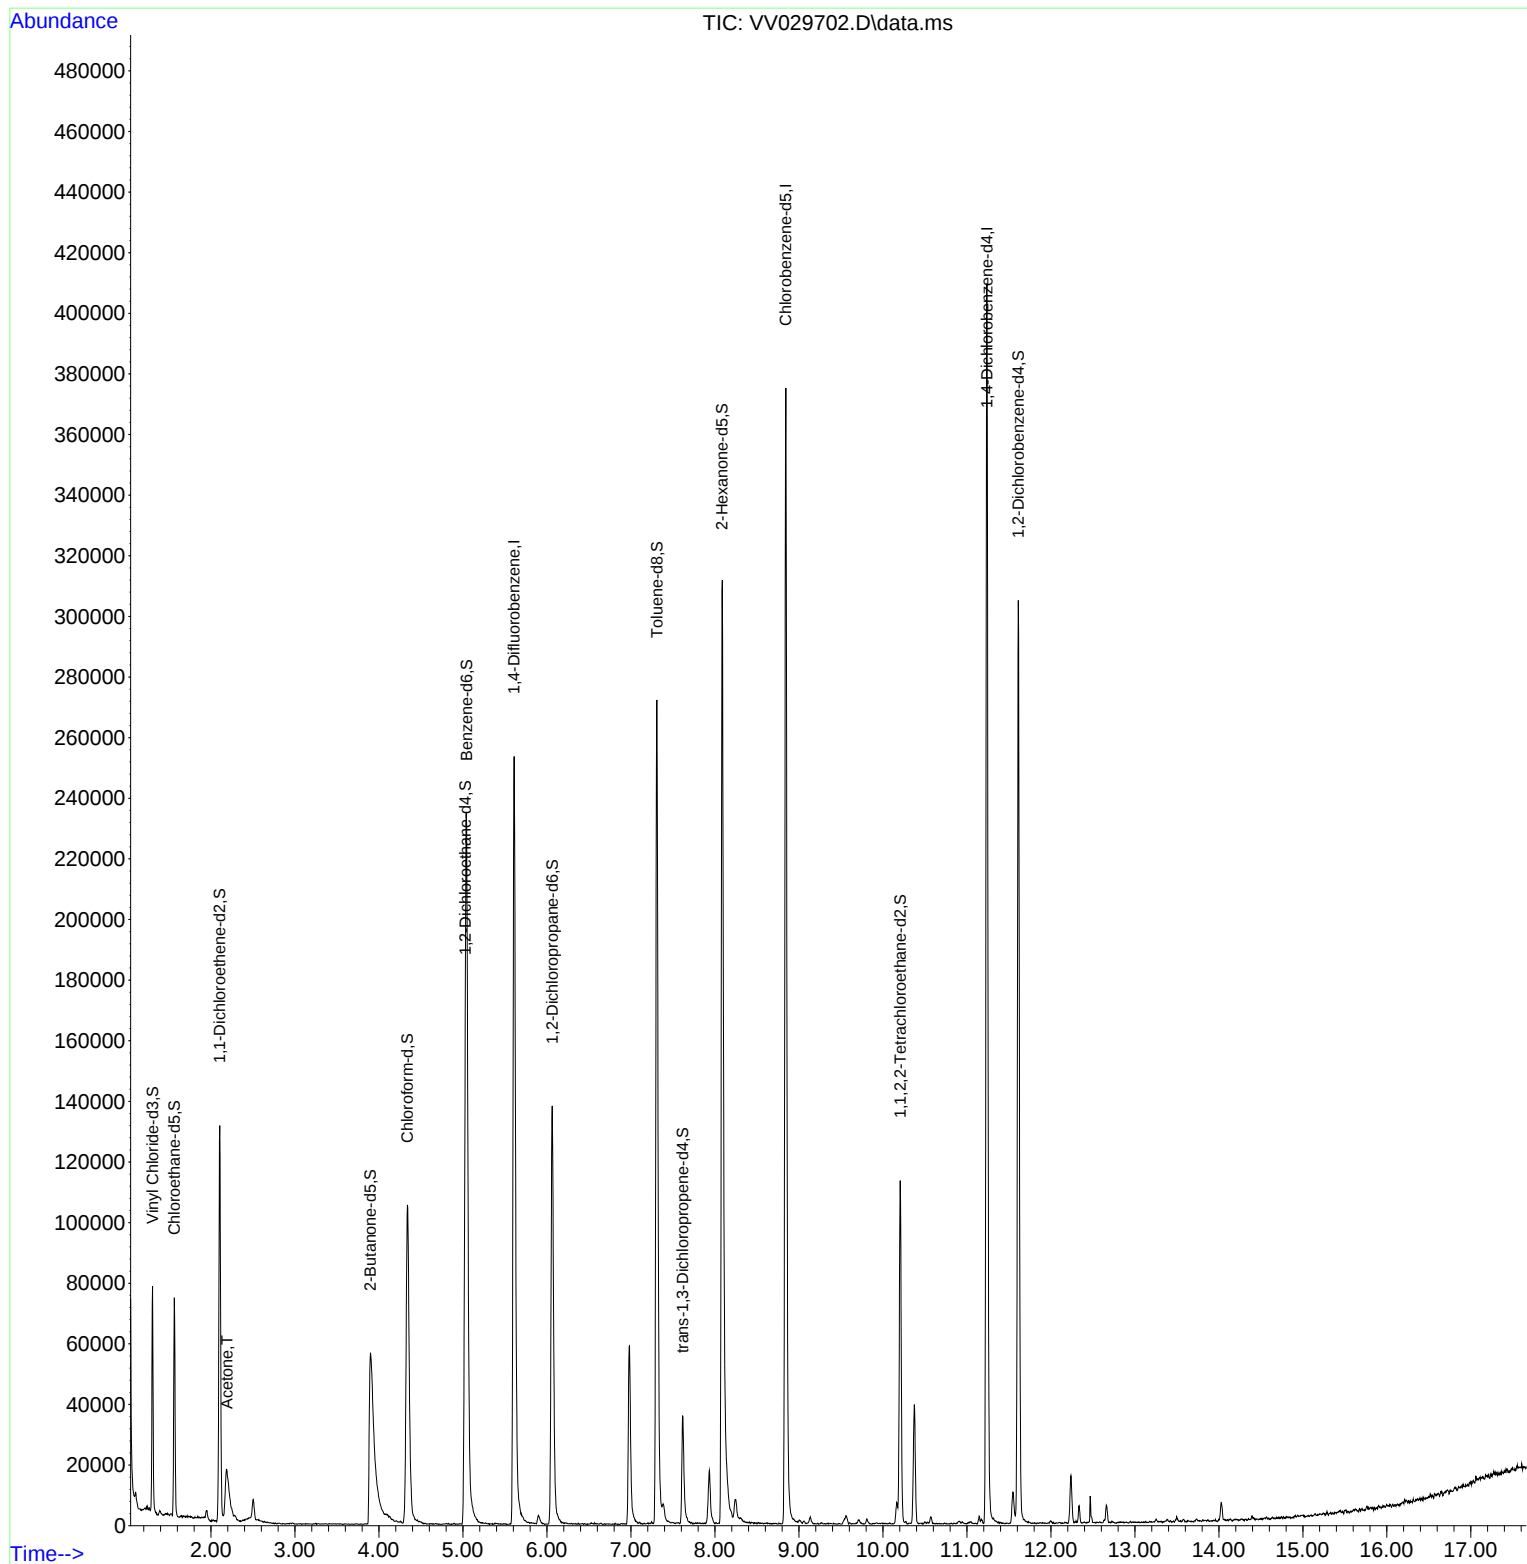

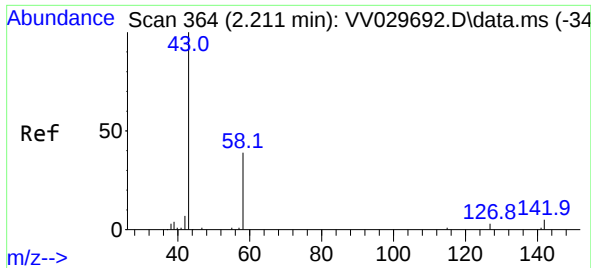

#13
Acetone
Concen: 19.761 ug/L
RT: 2.192 min Scan# 31
Delta R.T. -0.019 min
Lab File: VV029702.D
Acq: 16 Dec 2022 16:58

Instrument :
MSVOA_V
ClientSampleId :
BGPL4

Tgt Ion: 43 Resp: 35302
Ion Ratio Lower Upper
43 100
58 35.4 0.0 70.8

