

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
 Data File : VV029697.D
 Acq On : 16 Dec 2022 14:59
 Operator : SY/MD
 Sample : N6034-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGPK7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	70	rVB	46513	44754	6.94%	0.745%
2	1.304	76	82	99	rVB	85801	89022	13.79%	1.482%
3	1.388	102	108	113	rBV	6054	8162	1.26%	0.136%
4	1.564	156	163	175	rVB	78373	91572	14.19%	1.525%
5	2.105	320	331	346	rBV2	148616	220987	34.24%	3.679%
6	2.188	349	357	359	rBV3	5104	6967	1.08%	0.116%
7	2.767	526	537	548	rBV3	3898	8361	1.30%	0.139%
8	3.902	877	890	934	rBV2	62696	257941	39.97%	4.294%
9	4.342	1010	1027	1058	rBV3	113966	317885	49.26%	5.293%
10	5.040	1225	1244	1281	rBV2	250460	645323	100.00%	10.744%
11	5.609	1399	1421	1453	rBV	249506	518403	80.33%	8.631%
12	5.911	1502	1515	1534	rVB5	10865	24113	3.74%	0.401%
13	6.063	1549	1562	1583	rBV	149315	310660	48.14%	5.172%
14	6.982	1837	1848	1873	rBV2	64494	123221	19.09%	2.052%
15	7.310	1938	1950	1970	rBV	296374	534416	82.81%	8.898%
16	7.616	2035	2045	2064	rBV	39253	71159	11.03%	1.185%
17	7.937	2133	2145	2146	rBV	9546	13147	2.04%	0.219%
18	7.969	2146	2155	2172	rVB2	49766	88246	13.67%	1.469%
19	8.088	2180	2192	2225	rBV	322443	644157	99.82%	10.725%
20	8.844	2415	2427	2449	rBV	368419	607159	94.09%	10.109%
21	10.162	2829	2837	2841	rBV3	7239	10133	1.57%	0.169%
22	10.207	2841	2851	2871	rVB	120675	192298	29.80%	3.202%
23	10.374	2891	2903	2916	rVB	19001	31183	4.83%	0.519%
24	11.239	3160	3172	3197	rBV	399713	625992	97.00%	10.422%
25	11.612	3277	3288	3310	rBV	322310	513386	79.55%	8.547%
26	14.027	4028	4039	4050	rBV2	4403	7665	1.19%	0.128%




Sum of corrected areas: 6006312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029697.D
Acq On : 16 Dec 2022 14:59
Operator : SY/MD
Sample : N6034-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

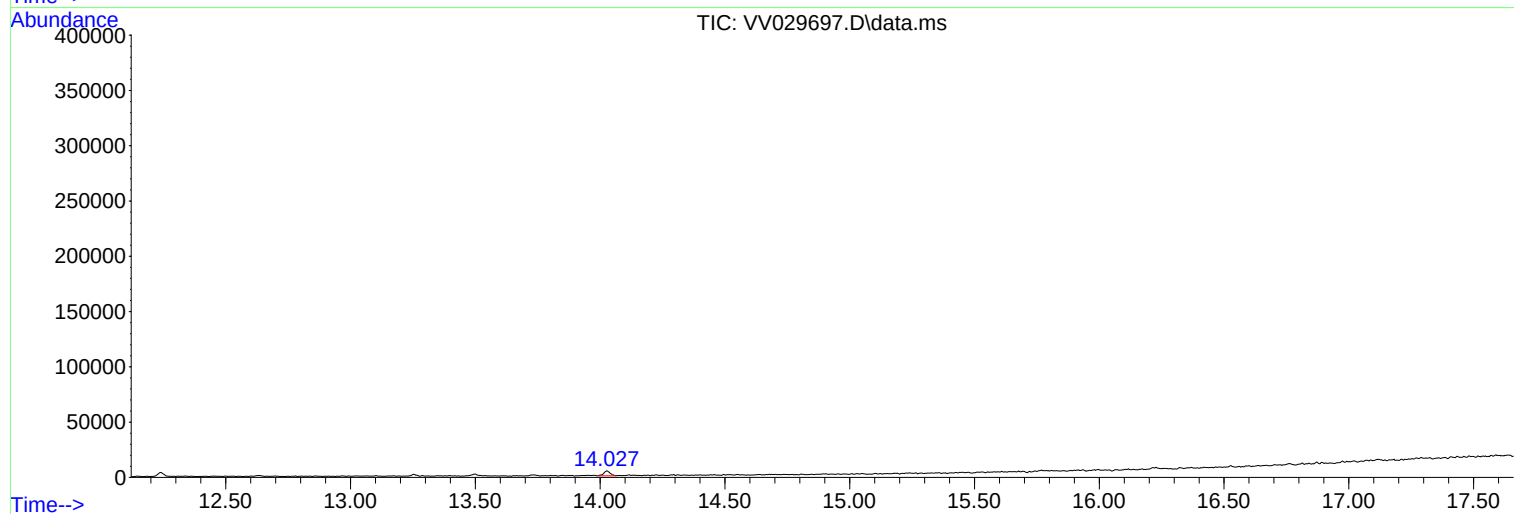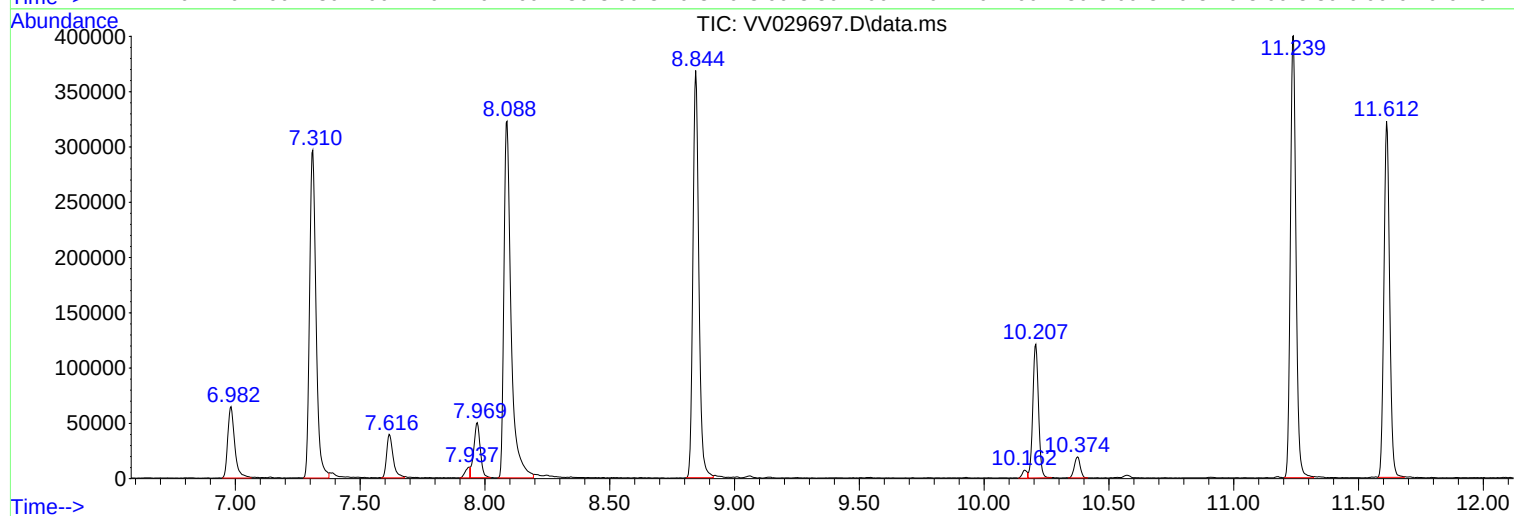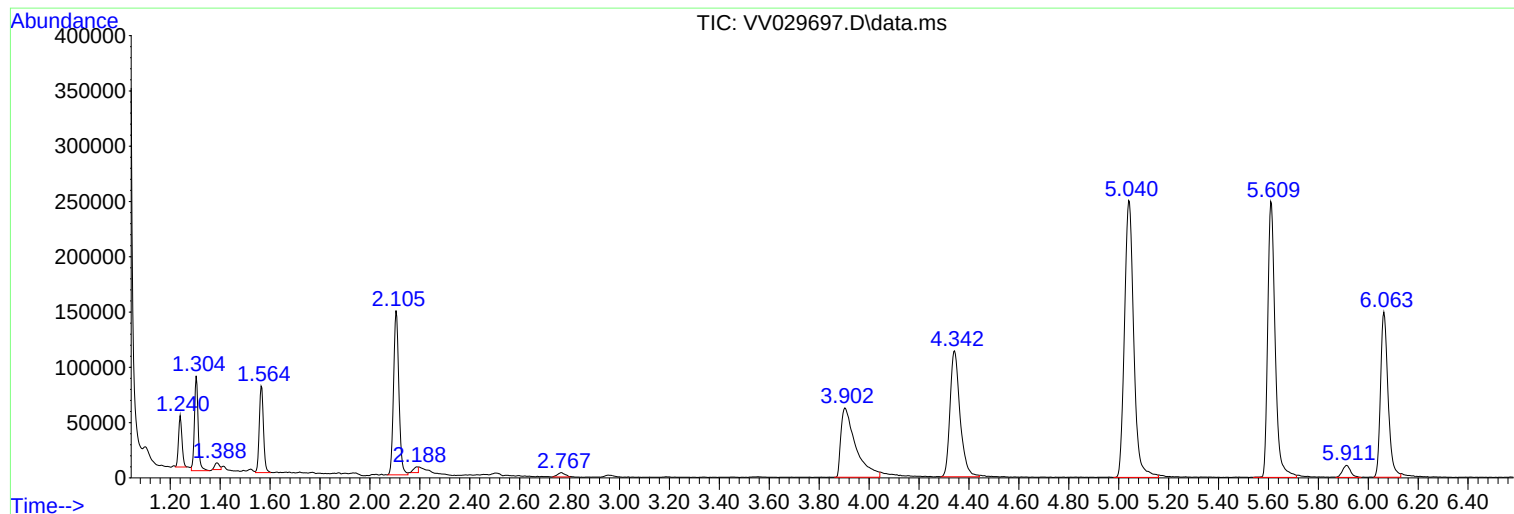

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029697.D
Acq On : 16 Dec 2022 14:59
Operator : SY/MD
Sample : N6034-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029697.D
Acq On : 16 Dec 2022 14:59
Operator : SY/MD
Sample : N6034-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
