

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
 Data File : VV029703.D
 Acq On : 16 Dec 2022 17:22
 Operator : SY/MD
 Sample : N6034-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGPL7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	27	rVB	6541	7153	1.02%	0.120%
2	1.304	75	82	94	rVB	77064	77837	11.10%	1.301%
3	1.564	155	163	177	rVB	73821	84334	12.03%	1.410%
4	2.104	318	331	345	rBV	132682	189594	27.05%	3.169%
5	2.191	346	358	379	rBV4	12142	45044	6.43%	0.753%
6	2.503	445	455	473	rVB2	8450	15153	2.16%	0.253%
7	3.905	880	891	937	rBV2	50726	239576	34.18%	4.005%
8	4.339	1010	1026	1050	rBV	105068	275906	39.36%	4.612%
9	5.040	1228	1244	1275	rBV2	237194	602576	85.97%	10.072%
10	5.609	1407	1421	1455	rBV	281961	583706	83.28%	9.757%
11	6.063	1549	1562	1593	rBV	141155	293965	41.94%	4.914%
12	6.982	1835	1848	1871	rBV	59537	114683	16.36%	1.917%
13	7.310	1938	1950	1968	rBV	271784	494150	70.50%	8.260%
14	7.616	2034	2045	2066	rBV	35549	66420	9.48%	1.110%
15	7.934	2132	2144	2154	rBV	17868	32323	4.61%	0.540%
16	8.088	2180	2192	2230	rBV	310611	635243	90.63%	10.618%
17	8.242	2233	2240	2256	rVB6	4166	9800	1.40%	0.164%
18	8.844	2415	2427	2450	rBV	414796	688791	98.27%	11.513%
19	10.168	2828	2839	2842	rBV4	5717	9354	1.33%	0.156%
20	10.207	2842	2851	2867	rVB	114226	182367	26.02%	3.048%
21	10.374	2890	2903	2916	rVB	42450	67551	9.64%	1.129%
22	11.239	3160	3172	3194	rBV	439731	700932	100.00%	11.716%
23	11.545	3256	3267	3277	rBV3	11395	22802	3.25%	0.381%
24	11.612	3277	3288	3310	rVB	305280	488072	69.63%	8.158%
25	12.239	3472	3483	3494	rBV2	13778	23554	3.36%	0.394%
26	12.336	3505	3513	3527	rVB3	12729	19651	2.80%	0.328%
27	12.660	3601	3614	3627	rBV4	7638	12071	1.72%	0.202%




Sum of corrected areas: 5982608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029703.D
Acq On : 16 Dec 2022 17:22
Operator : SY/MD
Sample : N6034-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

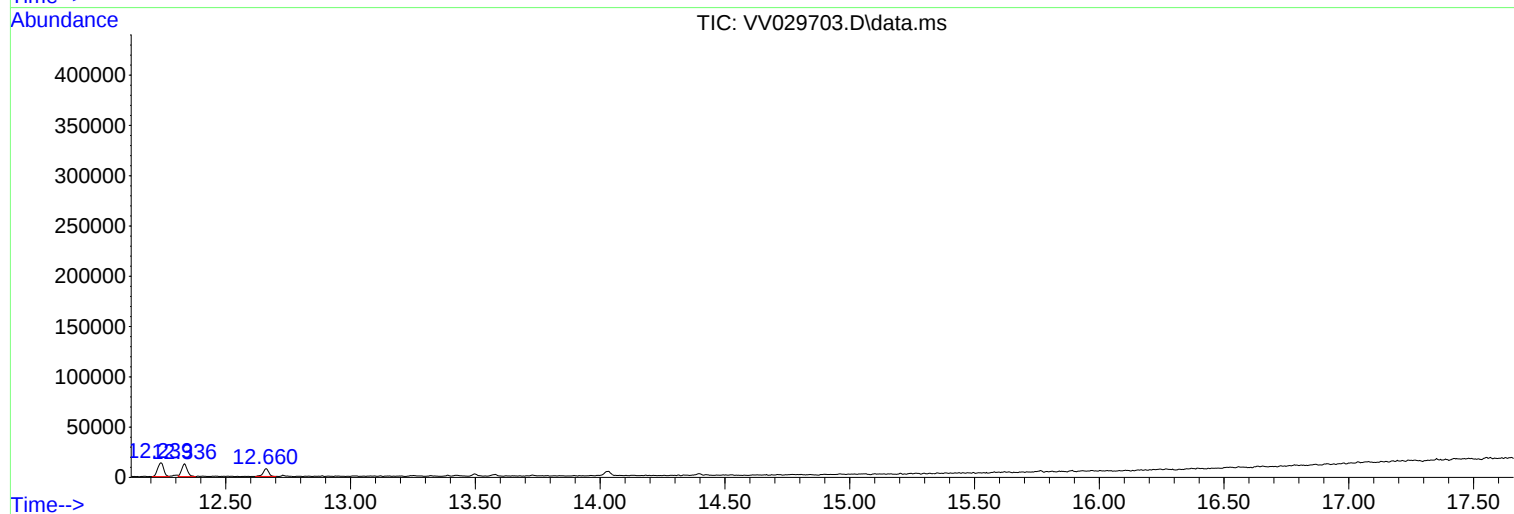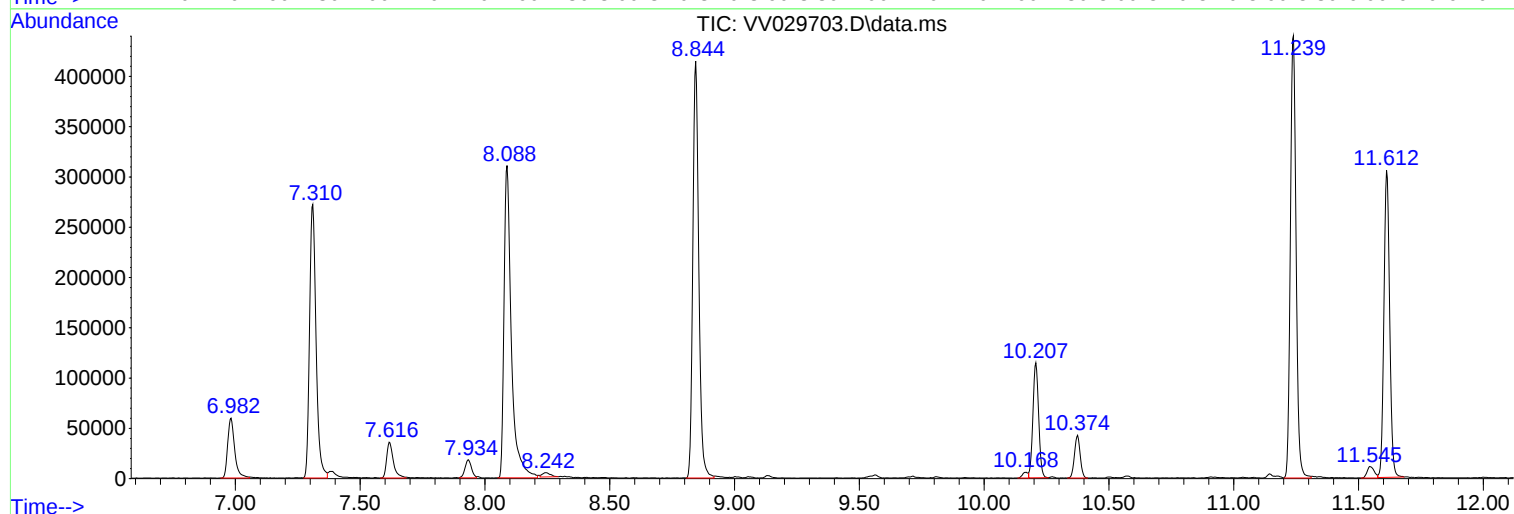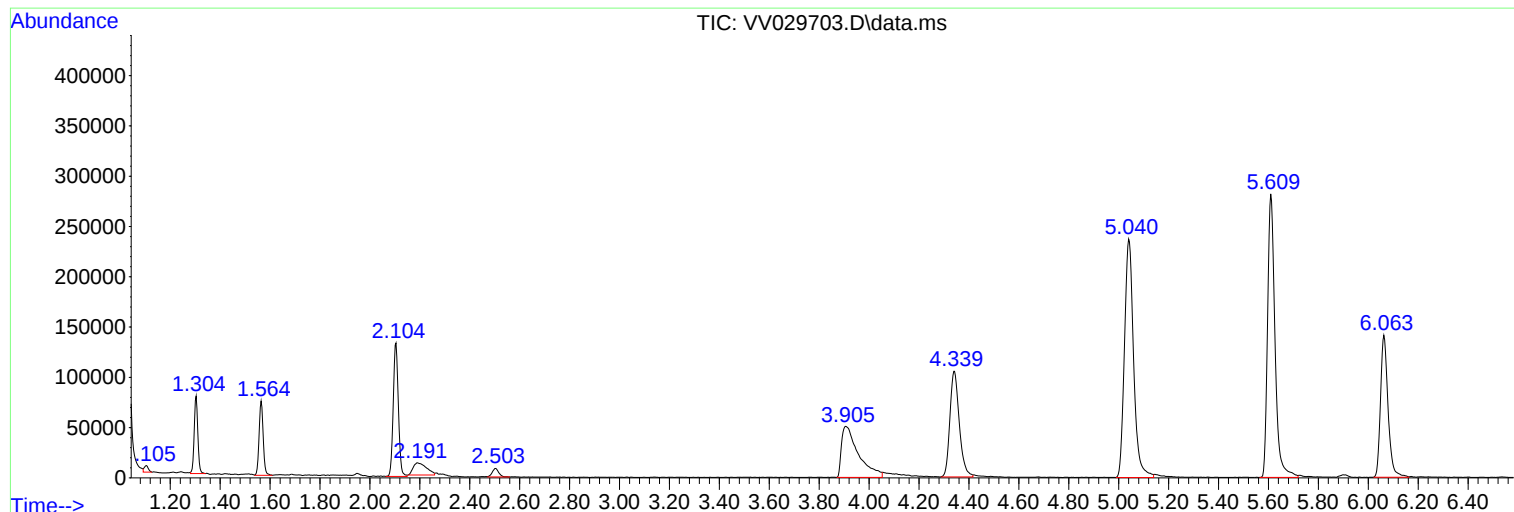

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029703.D
Acq On : 16 Dec 2022 17:22
Operator : SY/MD
Sample : N6034-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029703.D
Acq On : 16 Dec 2022 17:22
Operator : SY/MD
Sample : N6034-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGPL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------