

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
 Data File : VV029705.D
 Acq On : 16 Dec 2022 18:11
 Operator : SY/MD
 Sample : N6034-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	57	rBV	44144	38990	5.18%	0.633%
2	1.304	75	82	99	rVB	132619	135641	18.01%	2.201%
3	1.565	155	163	174	rBV	110637	122450	16.26%	1.987%
4	2.105	320	331	348	rBV	203144	293883	39.03%	4.769%
5	3.892	876	887	920	rBV2	60794	213168	28.31%	3.459%
6	4.339	1009	1026	1054	rBV2	124705	314887	41.82%	5.110%
7	5.040	1221	1244	1273	rBV2	295816	753003	100.00%	12.219%
8	5.609	1405	1421	1451	rBV	230668	482410	64.06%	7.828%
9	6.063	1548	1562	1590	rBV	165513	348347	46.26%	5.652%
10	6.979	1836	1847	1868	rBV2	73813	139763	18.56%	2.268%
11	7.310	1937	1950	1981	rBV	365174	666875	88.56%	10.821%
12	7.616	2035	2045	2066	rBV2	44610	80272	10.66%	1.303%
13	7.934	2134	2144	2153	rBV3	6457	12025	1.60%	0.195%
14	8.085	2181	2191	2229	rBV	311287	599511	79.62%	9.728%
15	8.844	2416	2427	2458	rBV	345454	576610	76.57%	9.356%
16	10.165	2829	2838	2841	rBV4	5563	7864	1.04%	0.128%
17	10.207	2841	2851	2866	rVB	119228	188569	25.04%	3.060%
18	10.371	2891	2902	2919	rVB2	13848	23115	3.07%	0.375%
19	11.239	3160	3172	3199	rBV	373069	590108	78.37%	9.575%
20	11.612	3276	3288	3312	rVB	357288	575234	76.39%	9.334%




Sum of corrected areas: 6162725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029705.D
Acq On : 16 Dec 2022 18:11
Operator : SY/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

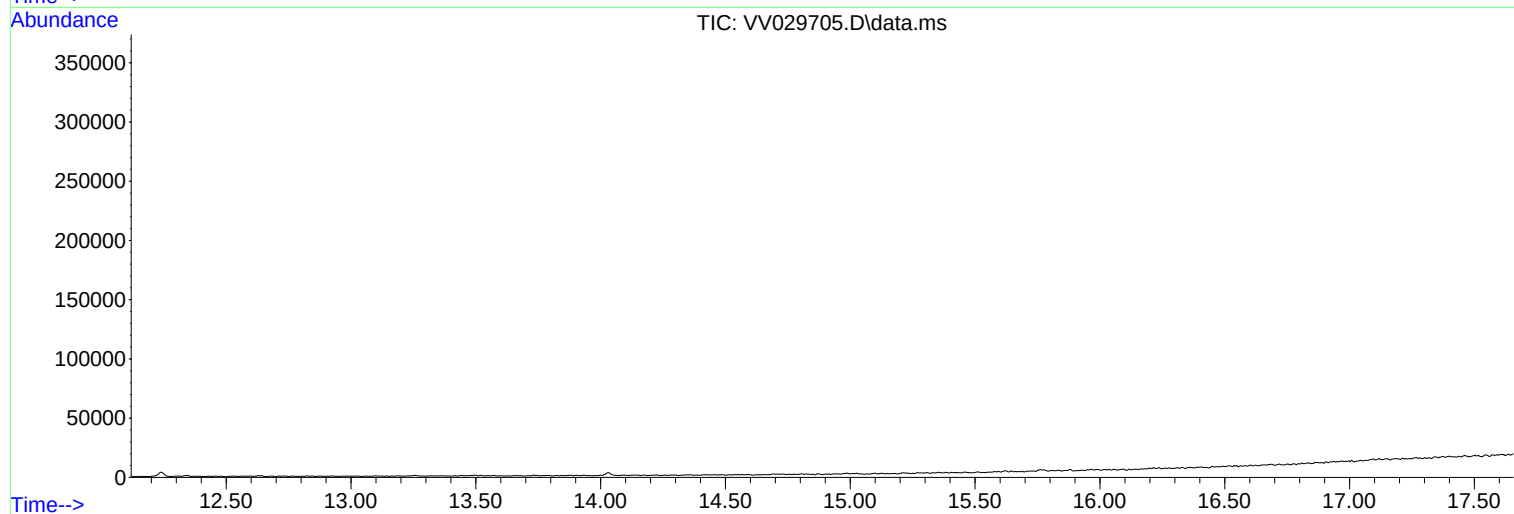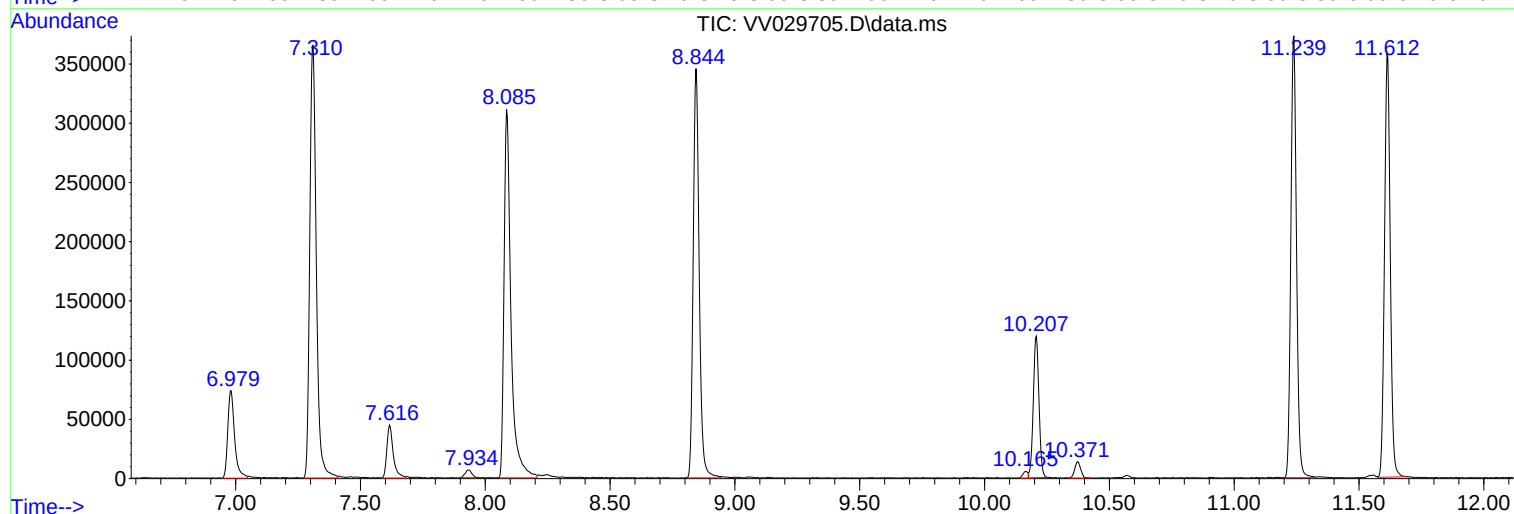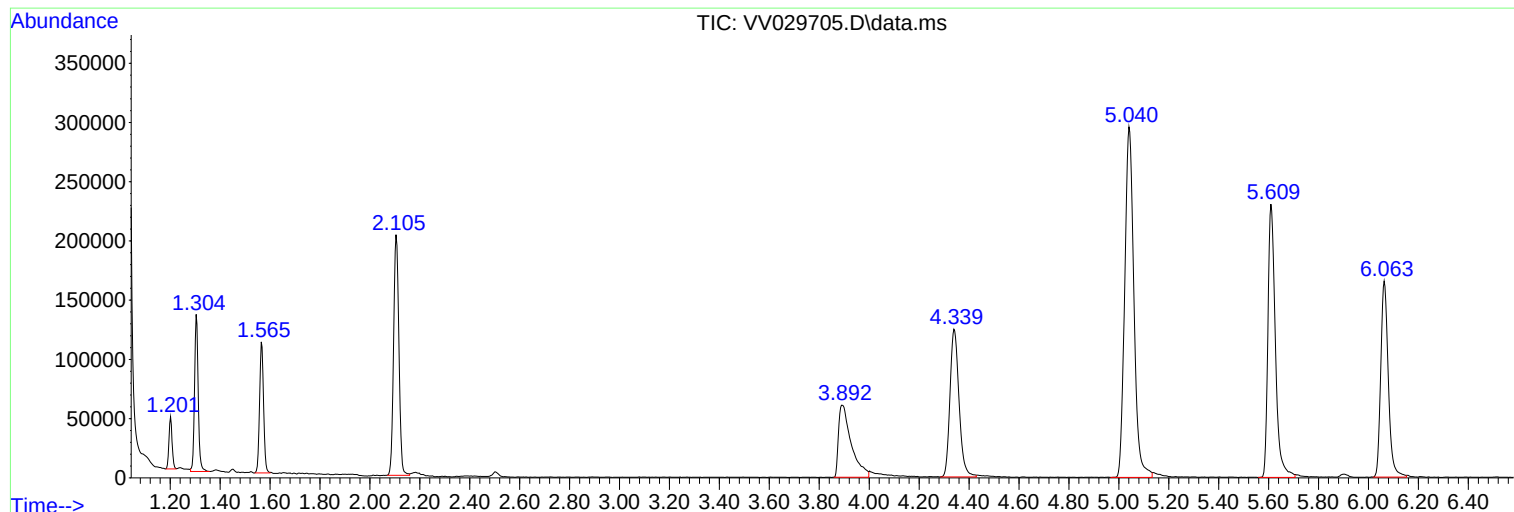

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029705.D
Acq On : 16 Dec 2022 18:11
Operator : SY/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
Data File : VV029705.D
Acq On : 16 Dec 2022 18:11
Operator : SY/MD
Sample : N6034-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc