


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121622\
 Data File : VV029691.D
 Acq On : 16 Dec 2022 09:03
 Operator : SY/MD
 Sample : BFB210
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB210

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Dec 16 20:17:28 2022

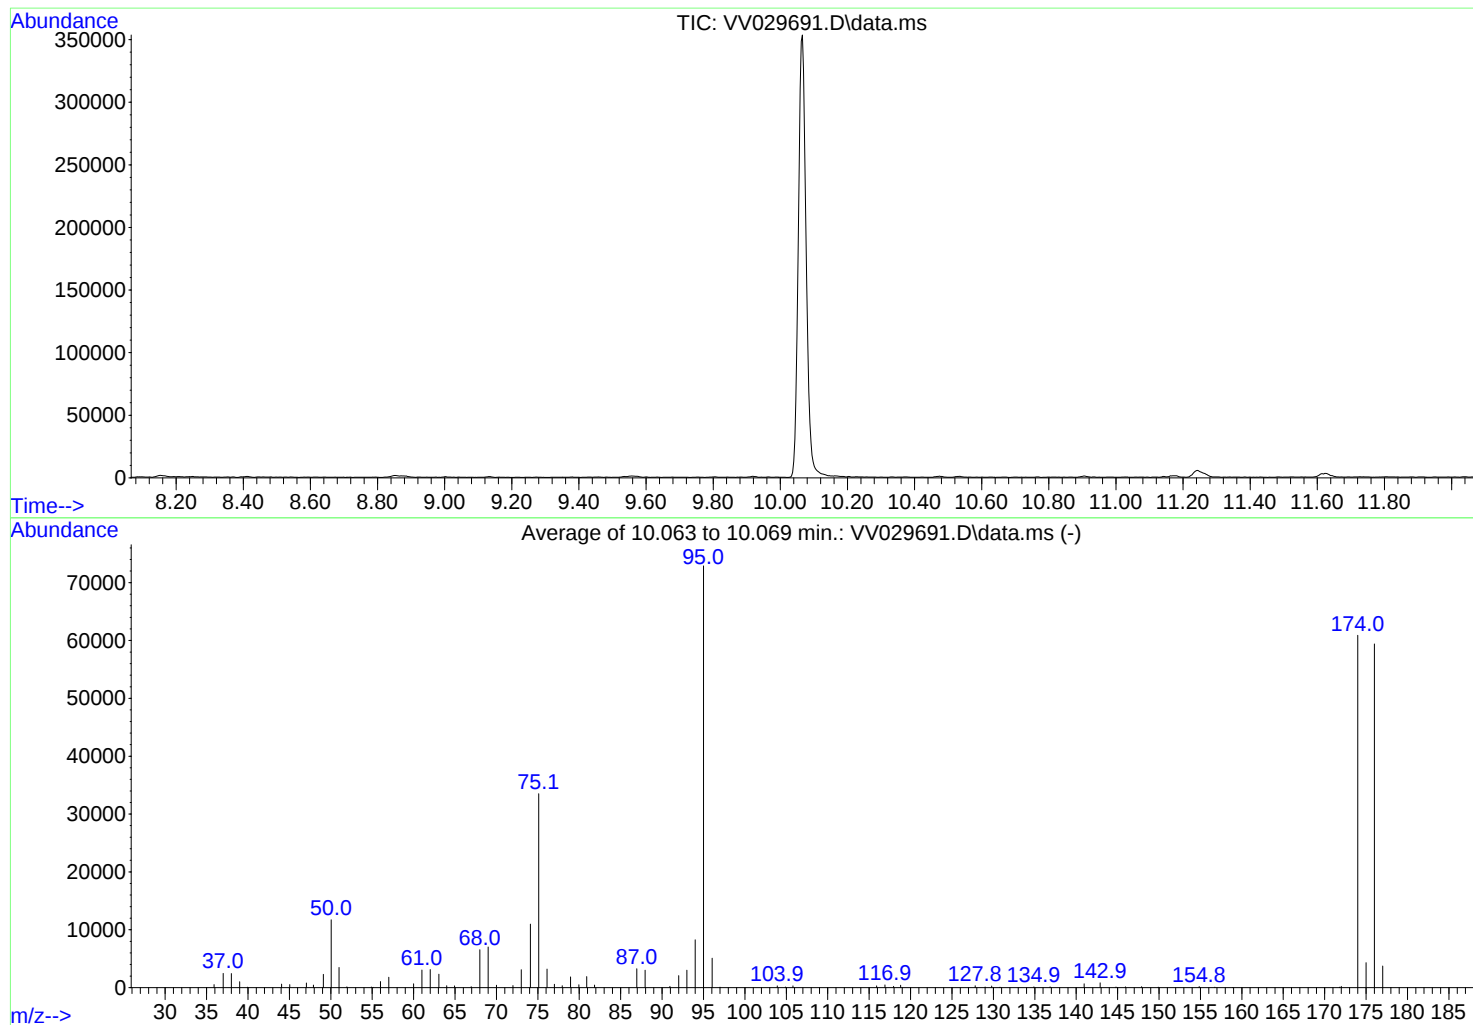

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	11724	PASS
75	95	30	80	46.0	33512	PASS
95	95	100	100	100.0	72901	PASS
96	95	5	9	7.0	5083	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	60893	PASS
175	174	5	9	7.1	4314	PASS
176	174	95	105	97.5	59400	PASS
177	176	5	10	6.3	3742	PASS

m/z	Abundance
39.90	144.0
43.80	278.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	552.0
37.00	2484.0
38.00	2402.0
39.00	1000.0
40.00	214.0
44.00	585.0
45.00	579.0
47.10	822.0
47.90	441.0
49.10	2288.0
50.00	12358.0
51.00	3717.0
52.00	154.0
54.90	187.0
56.00	1005.0
57.00	1852.0
60.00	697.0
61.00	3102.0
62.00	3287.0
63.00	2597.0
64.00	315.0
64.90	308.0
67.00	186.0
68.00	6722.0
69.00	7154.0
70.00	433.0
72.00	432.0
73.00	3111.0
74.10	11355.0
75.10	34392.0
76.10	3287.0
77.00	530.0
77.90	309.0
79.00	1848.0
80.00	482.0
80.90	1947.0
81.90	426.0
87.00	3621.0
87.90	3112.0
91.00	227.0
92.00	1988.0
93.00	3157.0
94.00	8472.0
95.00	74600.0
96.10	5182.0
97.00	104.0
103.90	280.0
104.90	129.0
105.80	312.0
115.90	331.0
116.90	480.0
117.90	220.0
118.80	426.0
127.80	298.0
129.10	114.0
129.80	278.0
130.80	118.0
134.90	140.0
136.90	146.0
140.90	611.0
142.90	784.0
144.70	115.0
146.00	132.0
147.90	173.0
154.80	192.0
156.80	156.0
171.80	276.0
174.00	61240.0
175.00	4294.0
176.00	59568.0
177.00	3797.0
178.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	539.0
37.00	2551.0
38.00	2473.0
39.00	1033.0
40.00	226.0
44.00	581.0
45.00	532.0
47.00	835.0
47.90	491.0
49.10	2337.0
50.00	12056.0
51.00	3580.0
52.00	143.0
54.90	171.0
56.00	1125.0
57.00	1851.0
60.00	706.0
61.00	3162.0
62.00	3200.0
63.10	2357.0
64.00	347.0
64.90	304.0
67.00	159.0
68.00	6745.0
69.00	7297.0
70.00	442.0
72.00	368.0
73.00	3204.0
74.10	11330.0
75.10	34736.0
76.10	3356.0
77.00	608.0
78.00	317.0
79.00	1880.0
80.00	529.0
80.90	1974.0
81.90	460.0
86.90	3327.0
88.00	3087.0
91.00	228.0
92.00	2175.0
93.00	3113.0
94.00	8558.0
95.00	75216.0
96.00	5303.0
103.90	319.0
104.90	125.0
105.80	322.0
115.90	293.0
116.90	512.0
118.00	219.0
118.80	448.0
127.80	339.0
129.00	112.0
129.80	291.0
130.80	104.0
134.90	149.0
136.80	163.0
140.90	706.0
142.90	851.0
144.80	114.0
145.90	145.0
147.90	182.0
149.90	104.0
154.80	194.0
156.70	129.0
158.90	101.0
172.00	313.0
174.00	62712.0
175.00	4446.0
176.00	61464.0
177.00	3836.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	463.0
37.00	2367.0
38.00	2397.0
39.00	1009.0
40.00	257.0
44.10	627.0
45.10	479.0
47.00	782.0
47.90	428.0
49.10	2233.0
50.10	10757.0
51.00	3172.0
51.90	166.0
55.10	157.0
56.00	1059.0
57.00	1669.0
60.00	591.0
61.00	2834.0
62.00	2896.0
63.10	2021.0
64.00	341.0
65.00	266.0
66.90	179.0
68.00	6194.0
69.00	6598.0
70.00	408.0
72.00	288.0
73.00	2955.0
74.10	10282.0
75.10	31408.0
76.10	3001.0
77.00	598.0
78.00	358.0
78.90	1792.0
79.90	510.0
80.90	1835.0
81.80	415.0
86.90	2869.0
88.00	2819.0
90.90	202.0
92.00	2062.0
93.00	2795.0
94.00	7776.0
95.00	68888.0
96.00	4765.0
97.00	119.0
103.90	310.0
104.90	111.0
105.80	276.0
115.90	272.0
116.90	455.0
118.00	223.0
118.80	420.0
127.80	333.0
128.90	109.0
129.80	258.0
134.90	136.0
136.80	144.0
141.00	662.0
142.90	844.0
144.90	102.0
145.90	130.0
147.90	154.0
149.90	112.0
154.90	170.0
172.00	329.0
174.00	58728.0
175.00	4201.0
176.00	57168.0
177.00	3593.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210