


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121718\
 Data File : VV008969.D
 Acq On : 17 Dec 2018 10:10
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 18 03:36:51 2018

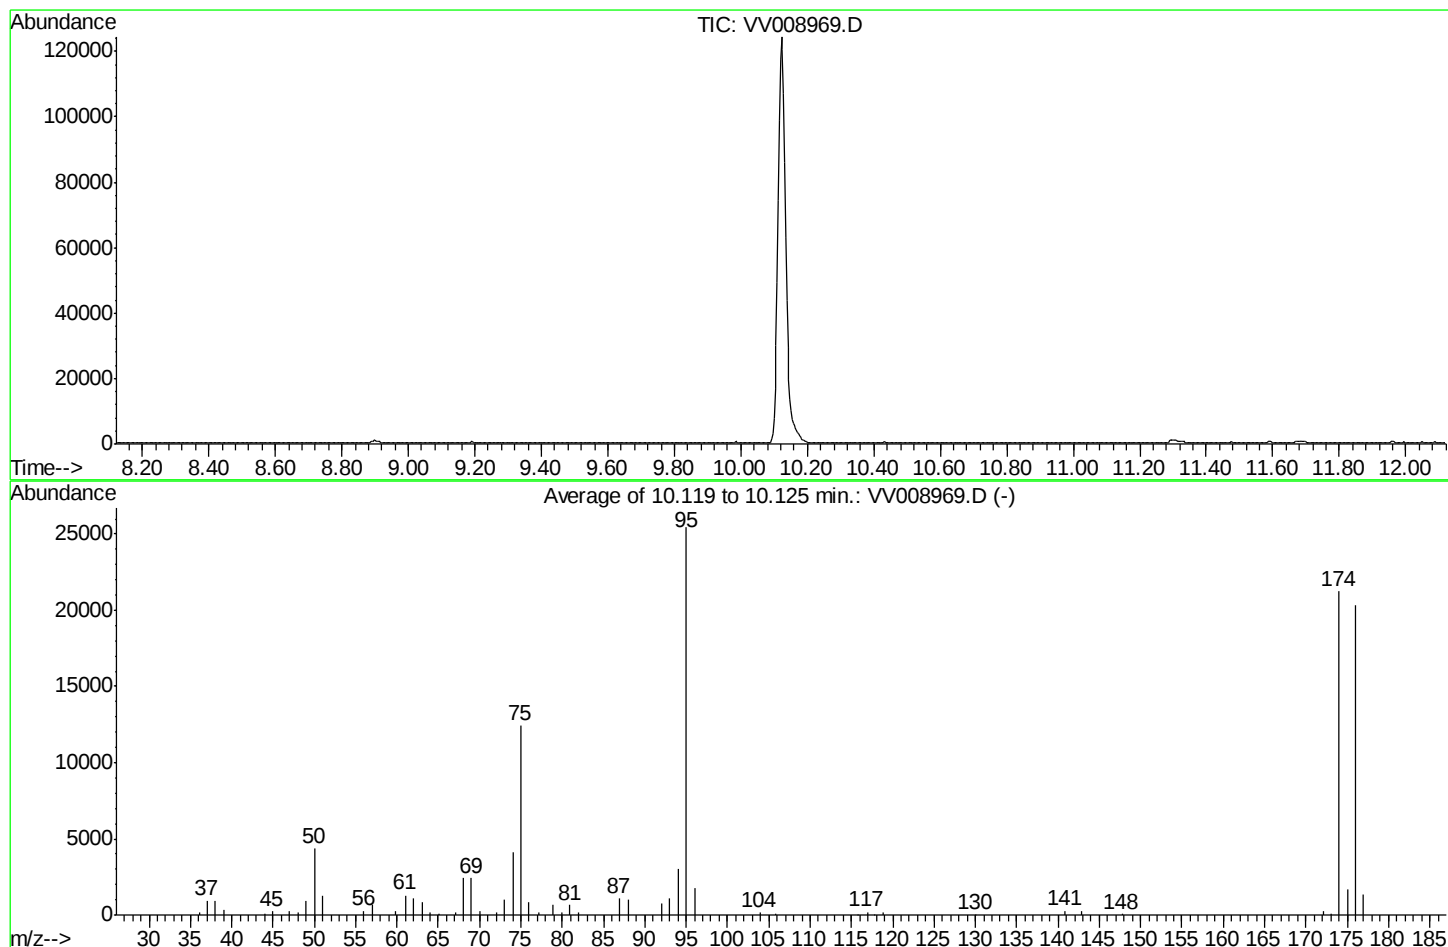

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4365	PASS
75	95	30	80	48.8	12418	PASS
95	95	100	100	100.0	25442	PASS
96	95	5	9	7.0	1787	PASS
173	174	0.00	2	0.6	123	PASS
174	95	50	120	83.5	21248	PASS
175	174	5	9	7.9	1680	PASS
176	174	95	101	95.7	20325	PASS
177	176	5	9	6.5	1315	PASS

m/z	Abundance
44.00	429.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	153.0
37.00	984.0
38.00	897.0
39.00	322.0
44.00	497.0
44.90	203.0
47.00	230.0
48.00	129.0
49.00	937.0
50.00	4474.0
50.90	1229.0
56.00	297.0
56.90	638.0
59.80	180.0
61.00	1273.0
62.00	1063.0
63.00	771.0
64.10	163.0
67.10	144.0
68.00	2270.0
69.00	2397.0
70.00	327.0
72.10	120.0
73.00	1086.0
74.00	3990.0
75.00	12381.0
76.00	782.0
77.10	182.0
78.90	651.0
80.00	186.0
80.90	598.0
81.90	173.0
86.90	994.0
88.00	1019.0
92.00	705.0
92.90	1033.0
94.00	2813.0
95.00	24736.0
96.00	1865.0
103.90	147.0
115.70	107.0
116.90	192.0
117.80	108.0
118.90	157.0
130.00	121.0
140.80	270.0
142.80	271.0
147.80	104.0
172.10	233.0
173.10	369.0
174.00	20152.0
175.00	1611.0
176.00	19200.0
177.00	1283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	165.0
37.00	977.0
38.00	1006.0
39.00	315.0
44.00	488.0
44.90	228.0
47.00	288.0
48.10	134.0
48.90	1002.0
50.00	4481.0
51.00	1283.0
56.00	269.0
56.90	665.0
59.90	214.0
61.00	1342.0
62.00	1142.0
63.00	886.0
64.10	133.0
65.00	107.0
67.10	156.0
68.00	2503.0
69.00	2477.0
70.00	285.0
72.10	174.0
73.00	1057.0
74.00	4167.0
75.00	12803.0
76.00	880.0
77.10	182.0
78.90	716.0
79.90	206.0
80.90	667.0
81.90	154.0
86.90	1135.0
88.00	1059.0
92.00	760.0
93.00	1096.0
94.00	3130.0
95.00	26128.0
96.00	1861.0
103.90	145.0
105.90	120.0
116.90	226.0
118.90	200.0
140.80	301.0
142.80	268.0
147.80	104.0
172.00	267.0
174.00	21936.0
175.00	1752.0
176.00	20960.0
177.00	1391.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.10	161.0
37.00	871.0
38.00	929.0
39.00	348.0
43.90	501.0
44.90	216.0
47.00	323.0
48.10	124.0
48.90	922.0
50.00	4141.0
51.00	1191.0
56.00	275.0
57.00	605.0
59.90	247.0
61.00	1222.0
62.00	1103.0
63.00	936.0
63.90	134.0
65.10	151.0
67.10	112.0
68.00	2435.0
69.00	2412.0
70.00	234.0
72.00	168.0
73.00	995.0
74.00	4116.0
75.00	12071.0
76.00	924.0
77.10	175.0
78.90	695.0
79.90	218.0
80.90	707.0
81.90	153.0
86.90	1059.0
88.00	947.0
92.00	711.0
92.90	1051.0
94.00	3073.0
95.00	25464.0
96.00	1637.0
103.90	122.0
105.90	119.0
116.90	201.0
118.90	236.0
140.90	284.0
142.90	250.0
172.00	246.0
174.00	21656.0
175.00	1677.0
176.00	20816.0
177.00	1271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99