
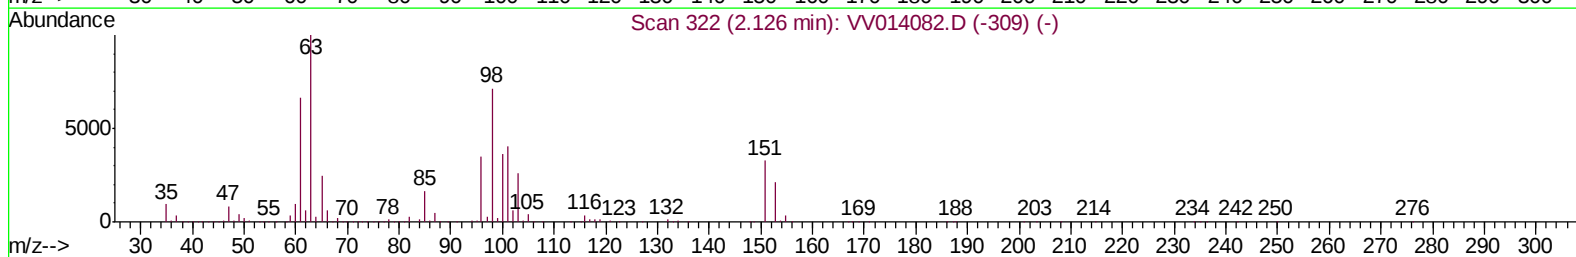
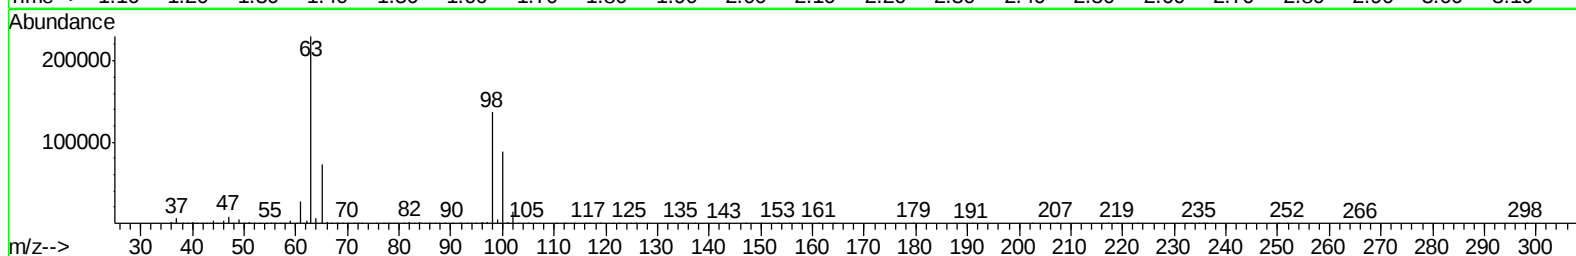


Data File : VV014093.D
Acq On : 17 Dec 2019 15:10
Operator : SY/MD
Sample : K6276-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 18 06:55:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 06:35:10 2019
Response via : Initial Calibration

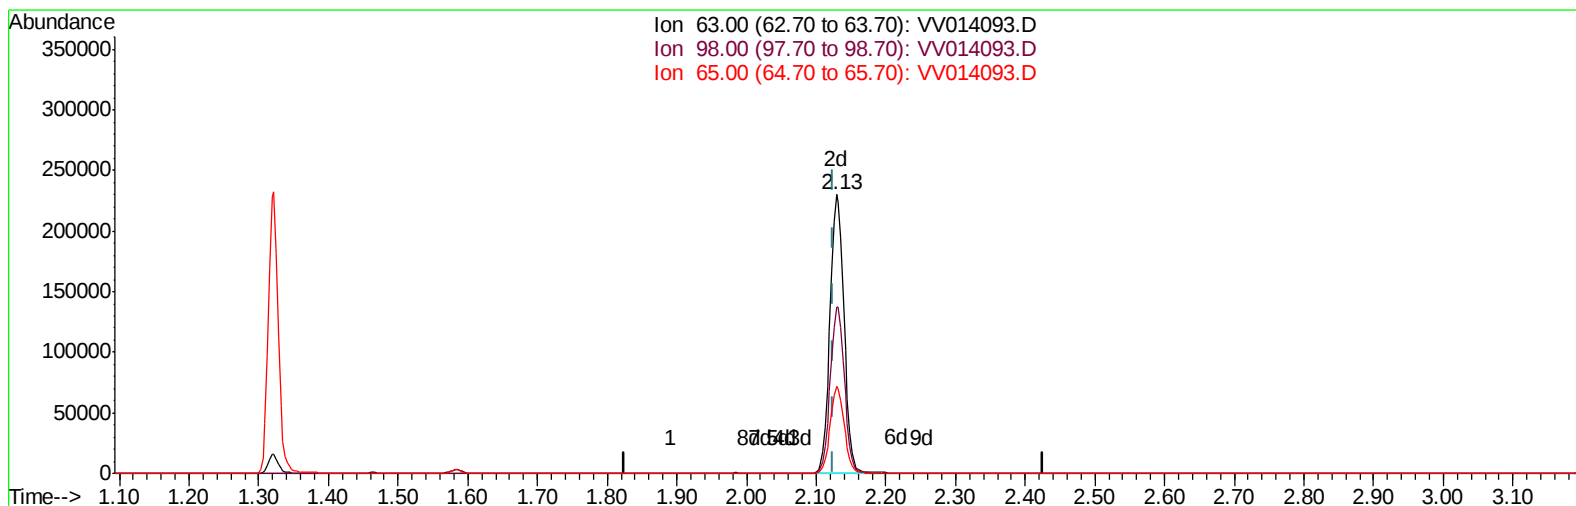

TIC: VV014093.D

(11) 1,1-Dichloroethene-d2 (S)

2.129min (+0.003) 34.76ug/L m

response 322732

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	0.01#
65.00	23.60	0.01#
0.00	0.00	0.00