
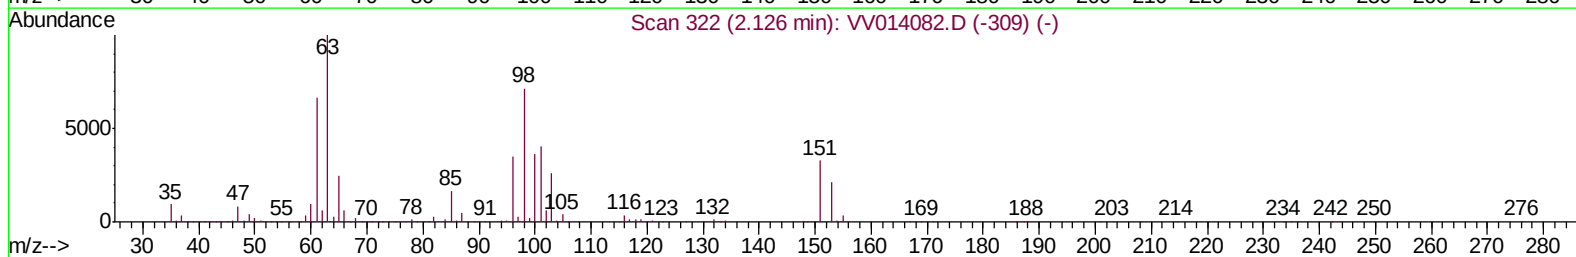
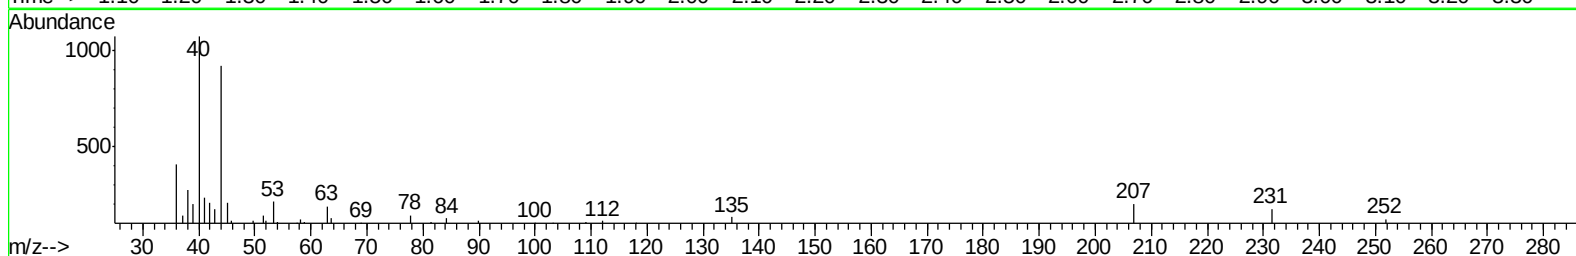


Data File : VV014095.D
Acq On : 17 Dec 2019 15:57
Operator : SY/MD
Sample : K6276-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 18 06:56:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 06:35:10 2019
Response via : Initial Calibration

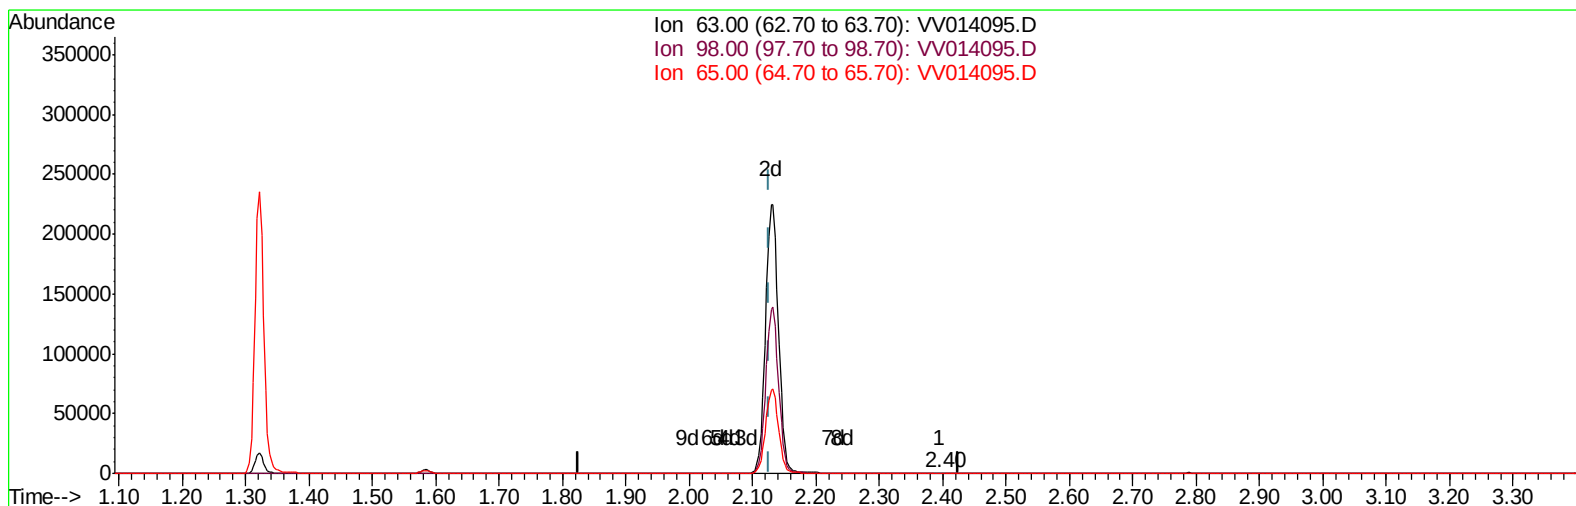

TIC: VV014095.D

(11) 1,1-Dichloroethene-d2 (S)

2.396min (+0.270) 0.02ug/L

response 176

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	63.64
65.00	23.60	25.00
0.00	0.00	0.00