
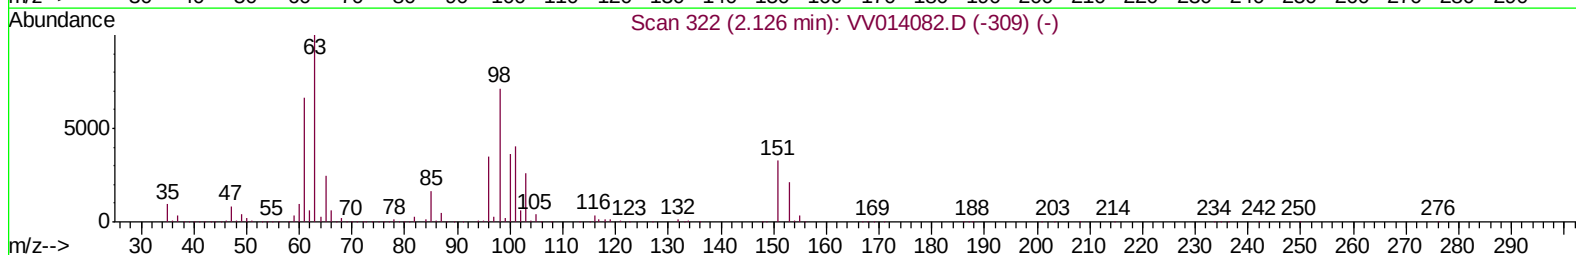
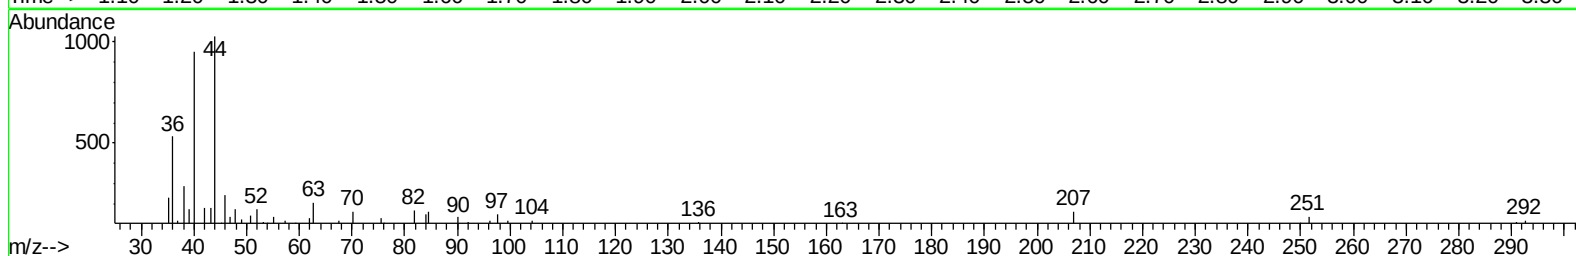


Data File : VV014102.D
Acq On : 17 Dec 2019 18:43
Operator : SY/MD
Sample : K6314-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 18 06:57:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 06:35:10 2019
Response via : Initial Calibration

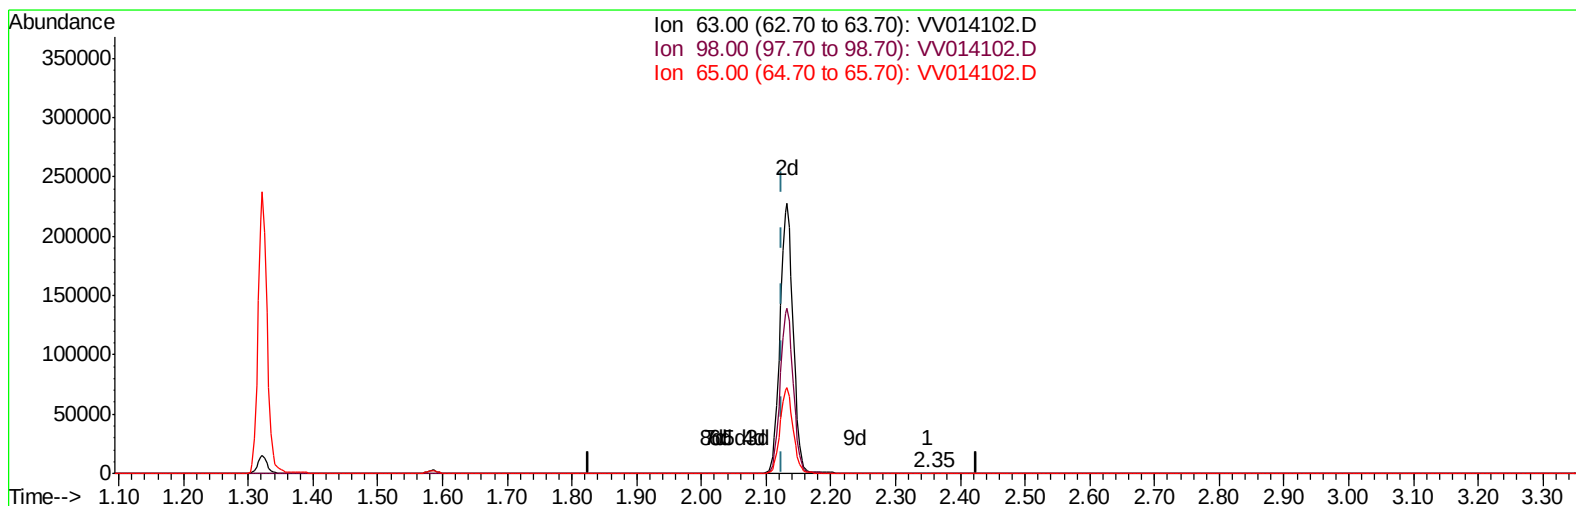

TIC: VV014102.D

(11) 1,1-Dichloroethene-d2 (S)

2.351min (+0.225) 0.02ug/L

response 163

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	55.83
65.00	23.60	25.77
0.00	0.00	0.00