
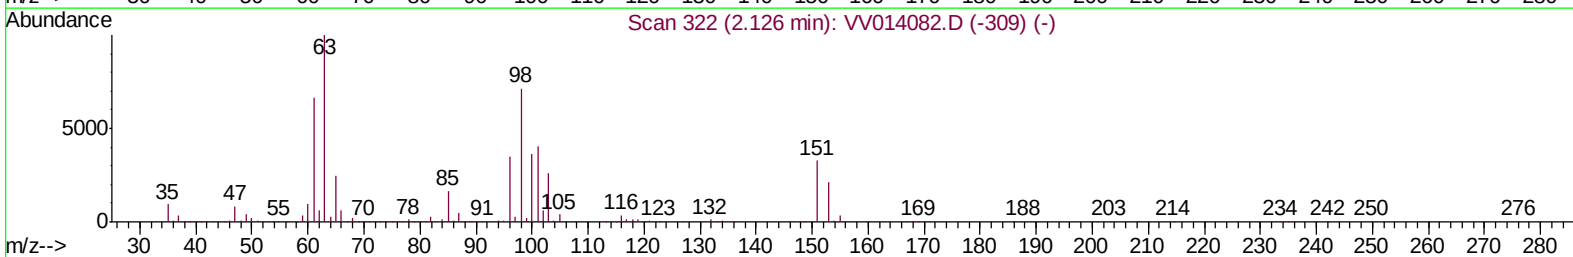
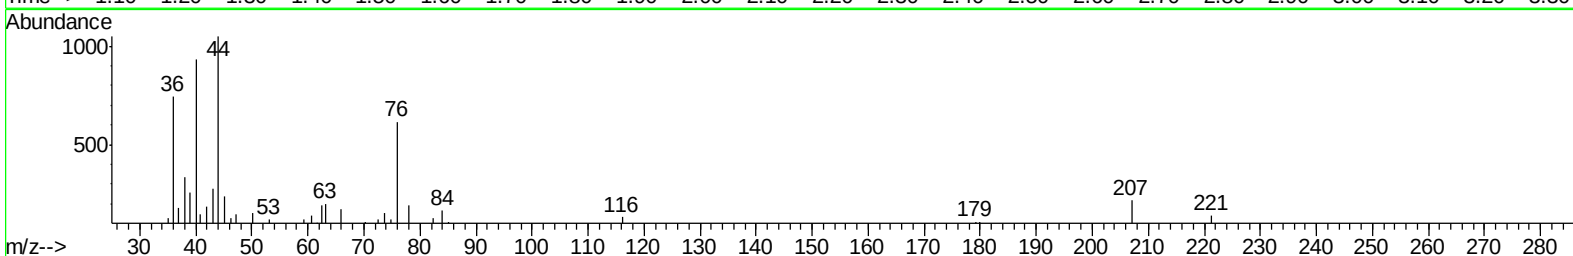


Data File : VV014103.D
Acq On : 17 Dec 2019 19:07
Operator : SY/MD
Sample : K6314-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 18 06:57:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 06:35:10 2019
Response via : Initial Calibration

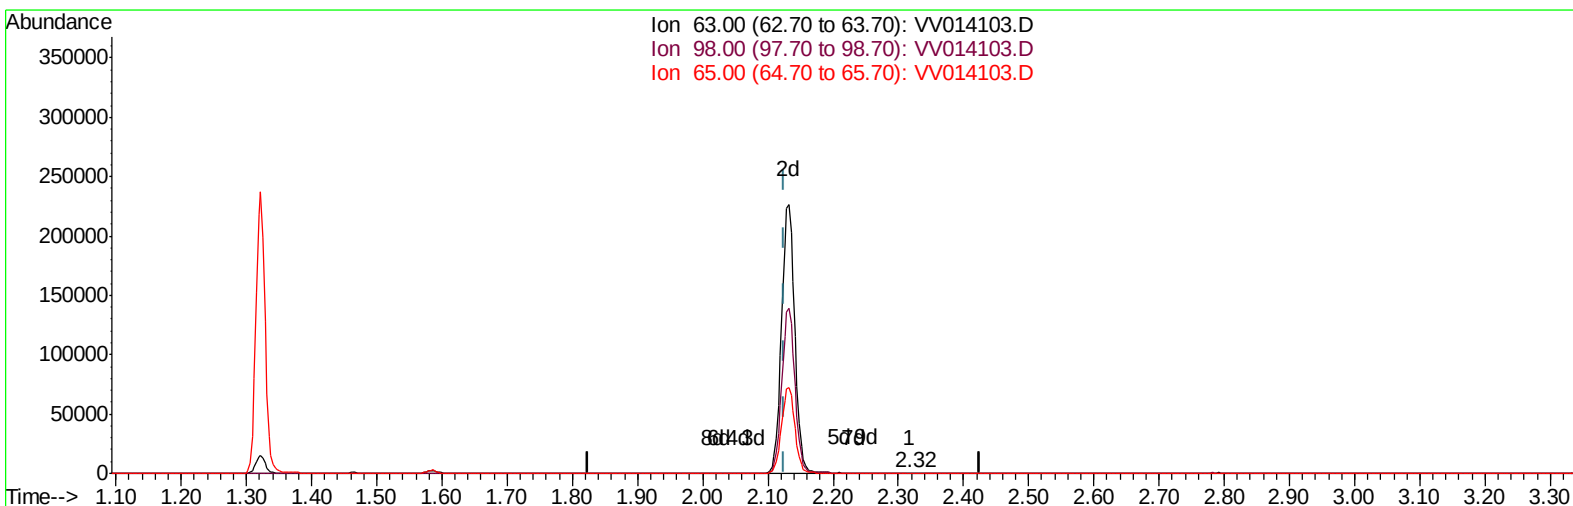

TIC: VV014103.D

(11) 1,1-Dichloroethene-d2 (S)

2.319min (+0.193) 0.02ug/L

response 207

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	61.35
65.00	23.60	22.71
0.00	0.00	0.00