

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014085.D
 Acq On : 17 Dec 2019 12:00
 Operator : SY/MD
 Sample : K6308-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C75

Quant Time: Dec 18 07:08:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 06:35:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	677675	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	684537	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	286429	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	251240	64.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	128.20%
7) Chloroethane-d5	1.58	69	231521	56.59	ug/L	0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	113.18%
11) 1,1-Dichloroethene-d2	2.13	63	339880	39.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.44%
21) 2-Butanone-d5	3.92	46	293345	106.34	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.34%
24) Chloroform-d	4.40	84	453974	55.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.32%
26) 1,2-Dichloroethane-d4	5.08	65	279443	53.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.16%
32) Benzene-d6	5.10	84	895340	50.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.96%
36) 1,2-Dichloropropane-d6	6.11	67	283604	53.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.52%
41) Toluene-d8	7.36	98	771800	47.73	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.46%
43) trans-1,3-Dichloropropene-	7.66	79	121350	46.84	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.68%
47) 2-Hexanone-d5	8.13	63	200066	100.63	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.63%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	380406	49.34	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.68%
64) 1,2-Dichlorobenzene-d4	11.67	152	305611	54.33	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.66%


Target Compounds					Ovalue
13) Acetone	2.18	43	10002	2.474 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014085.D
Acq On : 17 Dec 2019 12:00
Operator : SY/MD
Sample : K6308-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C75

Quant Time: Dec 18 07:08:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 06:35:10 2019
Response via : Initial Calibration

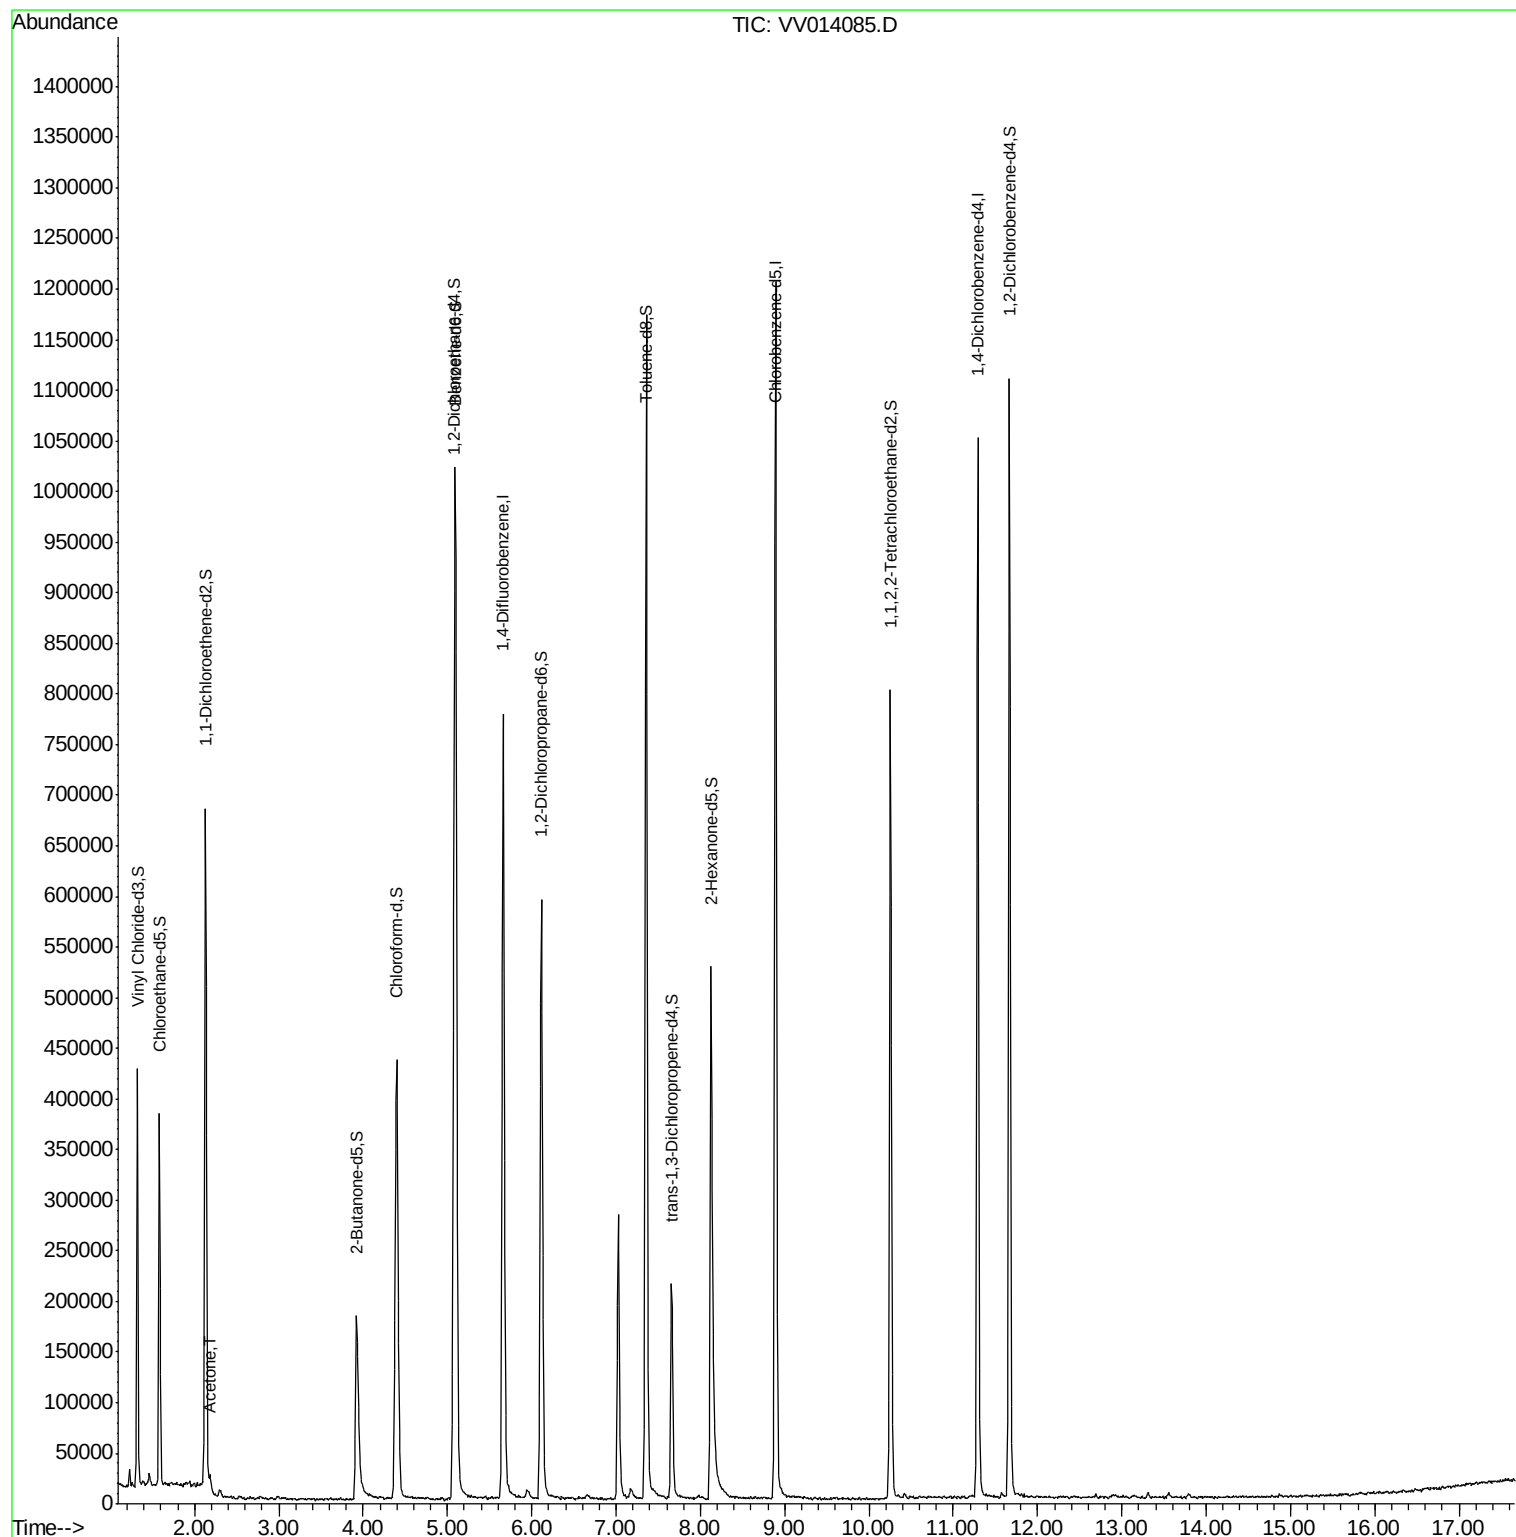

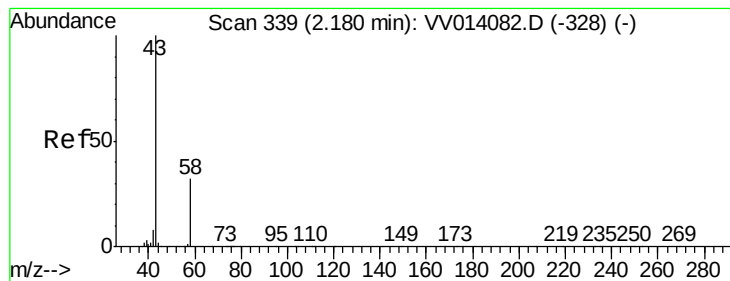

#13
 Acetone
 Concen: 2.474 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV014085.D
 Acq: 17 Dec 2019 12:00

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C75

Tot Ion: 43 Resp: 10002
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 60.8

