

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014084.D
 Acq On : 17 Dec 2019 11:37
 Operator : SY/MD
 Sample : K6308-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	39	43	48	rVB2	15364	14161	0.55%	0.073%
2	1.322	64	72	82	rBV	415428	417129	16.27%	2.142%
3	1.582	146	153	166	rVB	367612	406332	15.85%	2.087%
4	2.129	313	323	348	rVB	669797	985533	38.44%	5.061%
5	2.441	417	420	424	rBV5	1928	1444	0.06%	0.007%
6	2.460	424	426	431	rVB6	1847	1353	0.05%	0.007%
7	2.534	446	449	454	rVB7	3175	3158	0.12%	0.016%
8	2.557	454	456	459	rVB4	1958	1259	0.05%	0.006%
9	2.888	555	559	561	rBV5	1699	1310	0.05%	0.007%
10	2.907	561	565	570	rVB8	2589	2358	0.09%	0.012%
11	2.936	570	574	575	rBV4	1810	1443	0.06%	0.007%
12	3.068	610	615	620	rBV7	1991	2301	0.09%	0.012%
13	3.251	665	672	674	rBV7	1436	1323	0.05%	0.007%
14	3.624	784	788	790	rBV4	1577	1084	0.04%	0.006%
15	3.817	845	848	852	rVB7	1973	1255	0.05%	0.006%
16	3.843	852	856	861	rVB7	1811	1840	0.07%	0.009%
17	3.872	861	865	867	rBV3	1328	1199	0.05%	0.006%
18	3.917	867	879	905	rBV2	172541	458200	17.87%	2.353%
19	4.319	1001	1004	1006	rVB3	2129	1291	0.05%	0.007%
20	4.396	1006	1028	1051	rBV	432523	1079502	42.10%	5.543%
21	4.511	1062	1064	1068	rVB4	2281	1341	0.05%	0.007%
22	4.576	1082	1084	1087	rBV3	1890	1170	0.05%	0.006%
23	4.624	1094	1099	1102	rBV7	2879	2463	0.10%	0.013%
24	4.711	1120	1126	1130	rBV8	2682	2521	0.10%	0.013%
25	4.839	1163	1166	1170	rVB6	1418	1383	0.05%	0.007%
26	4.875	1170	1177	1178	rBV4	2041	2034	0.08%	0.010%
27	4.926	1191	1193	1198	rBV6	1611	1247	0.05%	0.006%
28	5.090	1226	1244	1271	rBV2	1011290	2564135	100.00%	13.167%
29	5.364	1327	1329	1334	rVB5	3300	2377	0.09%	0.012%
30	5.402	1337	1341	1342	rBV4	2637	1944	0.08%	0.010%
31	5.659	1406	1421	1442	rBV	813718	1629114	63.53%	8.366%
32	5.894	1492	1494	1500	rBV5	1704	1439	0.06%	0.007%
33	6.113	1546	1562	1580	rBV	572394	1160538	45.26%	5.960%
34	6.466	1671	1672	1679	rVB6	2274	1711	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014084.D
 Acq On : 17 Dec 2019 11:37
 Operator : SY/MD
 Sample : K6308-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.553	1694	1699	1700	rVV4	2483	1902	0.07%	0.010%
36	6.563	1700	1702	1706	rVV4	2421	2173	0.08%	0.011%
37	6.598	1710	1713	1716	rVV4	1804	1421	0.06%	0.007%
38	6.650	1723	1729	1734	rVV9	4872	7473	0.29%	0.038%
39	6.675	1735	1737	1740	rVV4	3220	1773	0.07%	0.009%
40	6.701	1741	1745	1748	rVB6	2097	1923	0.07%	0.010%
41	7.023	1833	1845	1864	rBV	275213	495643	19.33%	2.545%
42	7.267	1916	1921	1924	rBV6	2005	1770	0.07%	0.009%
43	7.354	1933	1948	1967	rBV	1139114	1965945	76.67%	10.096%
44	7.659	2032	2043	2058	rVV	206483	354473	13.82%	1.820%
45	7.785	2080	2082	2088	rBV7	1791	1206	0.05%	0.006%
46	7.971	2133	2140	2143	rBV8	3216	4317	0.17%	0.022%
47	8.055	2163	2166	2169	rVB5	1629	1061	0.04%	0.005%
48	8.126	2176	2188	2219	rBV	512861	1119888	43.68%	5.751%
49	8.650	2349	2351	2357	rVB7	2154	1737	0.07%	0.009%
50	8.704	2366	2368	2372	rBV5	1570	1359	0.05%	0.007%
51	8.794	2392	2396	2401	rVB7	1948	2103	0.08%	0.011%
52	8.830	2403	2407	2412	rVB8	2150	1811	0.07%	0.009%
53	8.891	2412	2426	2454	rBV	1242434	2050111	79.95%	10.528%
54	9.074	2481	2483	2488	rBV6	1394	1086	0.04%	0.006%
55	9.170	2511	2513	2516	rBV3	1934	1348	0.05%	0.007%
56	9.203	2521	2523	2530	rVB7	2234	1971	0.08%	0.010%
57	9.277	2543	2546	2554	rVB9	1716	1956	0.08%	0.010%
58	9.322	2554	2560	2563	rBV6	2408	2613	0.10%	0.013%
59	9.569	2634	2637	2639	rBV3	1656	1169	0.05%	0.006%
60	9.598	2644	2646	2649	rBV3	1435	1159	0.05%	0.006%
61	9.740	2689	2690	2696	rVB6	1549	1056	0.04%	0.005%
62	9.791	2703	2706	2709	rVV5	1779	1124	0.04%	0.006%
63	9.807	2709	2711	2717	rVB6	1183	1260	0.05%	0.006%
64	9.871	2728	2731	2733	rBV4	1540	1062	0.04%	0.005%
65	9.907	2740	2742	2746	rVB4	2125	1248	0.05%	0.006%
66	9.933	2746	2750	2757	rVB8	2103	2942	0.11%	0.015%
67	9.974	2757	2763	2765	rBV5	2799	3033	0.12%	0.016%
68	10.023	2775	2778	2781	rVB4	1862	1360	0.05%	0.007%
69	10.045	2781	2785	2789	rVB7	1745	1672	0.07%	0.009%
70	10.254	2838	2850	2870	rBV	779444	1232702	48.07%	6.330%
71	10.534	2934	2937	2939	rBV4	1774	1226	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014084.D
 Acq On : 17 Dec 2019 11:37
 Operator : SY/MD
 Sample : K6308-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.859	3033	3038	3039	rBV3	1519	1135	0.04%	0.006%
73	11.196	3140	3143	3144	rBV2	2510	1348	0.05%	0.007%
74	11.289	3159	3172	3192	rBV	1066366	1658800	64.69%	8.518%
75	11.666	3276	3289	3308	rBV	1080570	1715110	66.89%	8.807%
76	11.887	3355	3358	3360	rBV4	2566	1390	0.05%	0.007%
77	11.948	3375	3377	3380	rVB4	2341	1028	0.04%	0.005%
78	12.074	3413	3416	3420	rBV4	2078	1377	0.05%	0.007%
79	12.183	3448	3450	3453	rVB3	1729	1028	0.04%	0.005%
80	12.254	3469	3472	3478	rBV5	2103	2516	0.10%	0.013%
81	12.389	3511	3514	3517	rBV5	1839	1170	0.05%	0.006%
82	12.575	3570	3572	3576	rVB4	1850	1203	0.05%	0.006%
83	12.688	3603	3607	3613	rVB8	3441	3922	0.15%	0.020%
84	13.051	3718	3720	3725	rVB4	1835	1023	0.04%	0.005%
85	13.309	3794	3800	3812	rVB4	6779	11995	0.47%	0.062%
86	13.360	3812	3816	3818	rBV5	2299	1628	0.06%	0.008%
87	13.508	3860	3862	3867	rBV6	1354	1091	0.04%	0.006%
88	13.553	3867	3876	3884	rBV3	7810	13711	0.53%	0.070%
89	13.611	3891	3894	3897	rBV3	1730	1159	0.05%	0.006%
90	13.788	3944	3949	3950	rBV4	3331	2625	0.10%	0.013%
91	13.984	4005	4010	4014	rBV7	2124	2294	0.09%	0.012%
92	14.145	4056	4060	4061	rBV4	1370	1103	0.04%	0.006%
93	14.183	4068	4072	4073	rBV3	1758	1017	0.04%	0.005%
94	14.415	4136	4144	4149	rBV3	2436	3374	0.13%	0.017%
95	14.566	4189	4191	4193	rVB3	2847	1127	0.04%	0.006%
96	14.817	4266	4269	4272	rBV5	1771	1099	0.04%	0.006%
97	14.836	4272	4275	4278	rVV3	2021	1283	0.05%	0.007%
98	15.058	4341	4344	4348	rVB5	2155	1353	0.05%	0.007%
99	15.347	4432	4434	4437	rBV5	1899	1361	0.05%	0.007%
100	15.797	4571	4574	4576	rBV4	2000	1218	0.05%	0.006%


Sum of corrected areas: 19473456

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014084.D
Acq On : 17 Dec 2019 11:37
Operator : SY/MD
Sample : K6308-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

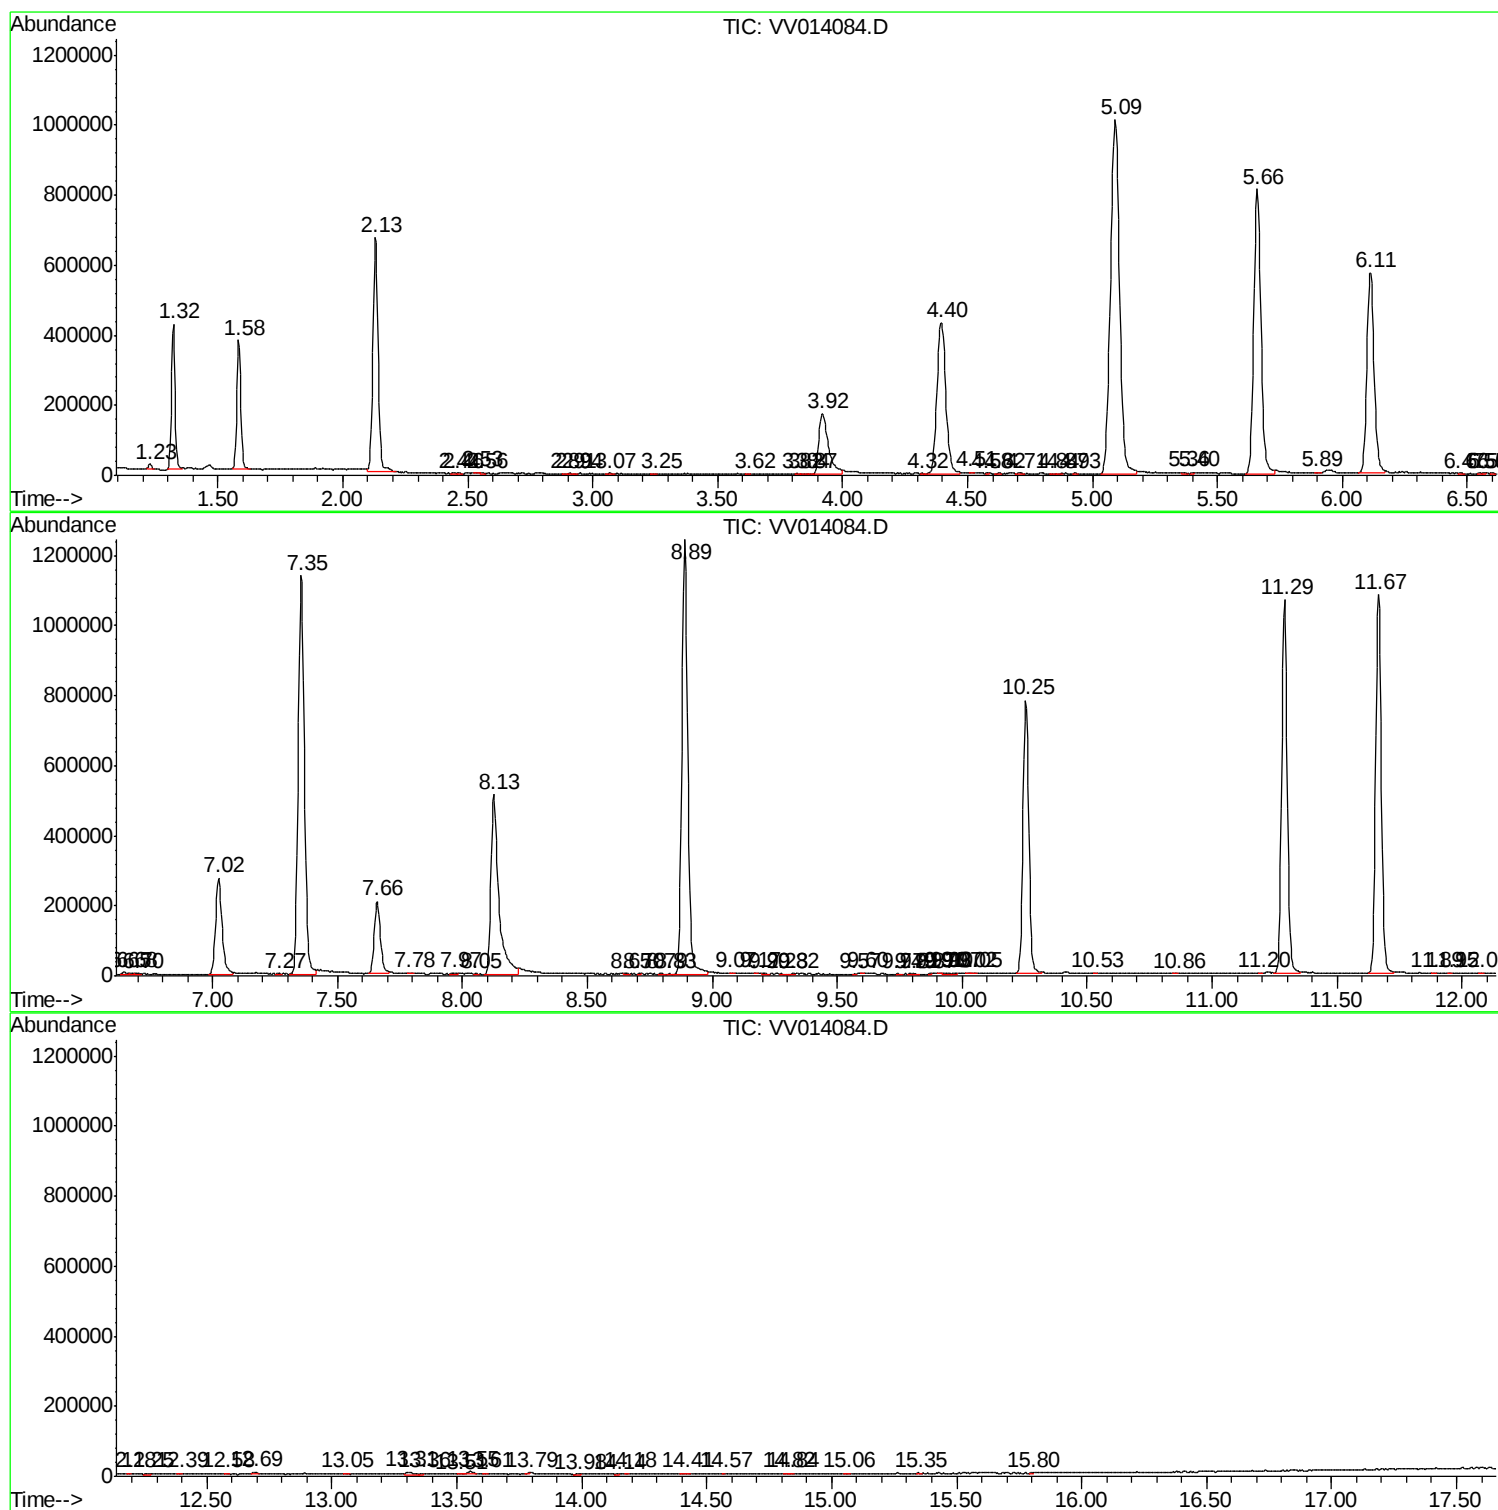

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014084.D
Acq On : 17 Dec 2019 11:37
Operator : SY/MD
Sample : K6308-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C81

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121719\
Data File : VV014084.D
Acq On : 17 Dec 2019 11:37
Operator : SY/MD
Sample : K6308-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0C81

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc