

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014085.D
 Acq On : 17 Dec 2019 12:00
 Operator : SY/MD
 Sample : K6308-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	40	43	49	rVB	17295	14407	0.55%	0.074%
2	1.322	64	72	84	rBV	412960	415947	15.87%	2.127%
3	1.582	146	153	167	rVB	366276	411031	15.68%	2.102%
4	2.132	314	324	335	rBV	665950	941182	35.91%	4.813%
5	2.524	441	446	448	rBV6	2778	2479	0.09%	0.013%
6	2.553	453	455	458	rVV4	2541	1450	0.06%	0.007%
7	2.630	473	479	482	rBV8	1946	2092	0.08%	0.011%
8	2.663	482	489	493	rBV10	2431	3213	0.12%	0.016%
9	2.698	498	500	505	rVB5	1835	1111	0.04%	0.006%
10	2.888	555	559	561	rBV4	1294	1028	0.04%	0.005%
11	2.901	561	563	566	rBV3	1809	1065	0.04%	0.005%
12	2.968	581	584	585	rBV3	1589	1030	0.04%	0.005%
13	3.048	606	609	612	rVB4	1939	1304	0.05%	0.007%
14	3.100	623	625	631	rVB6	1390	1176	0.04%	0.006%
15	3.135	631	636	638	rBV4	1800	1532	0.06%	0.008%
16	3.251	667	672	675	rBV4	1193	1025	0.04%	0.005%
17	3.312	689	691	694	rVB4	1805	1186	0.05%	0.006%
18	3.341	694	700	703	rBV7	1714	1691	0.06%	0.009%
19	3.441	729	731	737	rBV6	2119	2177	0.08%	0.011%
20	3.556	765	767	770	rVV4	1807	1392	0.05%	0.007%
21	3.569	770	771	775	rVV4	1974	1253	0.05%	0.006%
22	3.598	777	780	785	rVV7	1627	1654	0.06%	0.008%
23	3.618	785	786	790	rVB3	2155	1194	0.05%	0.006%
24	3.653	795	797	800	rBV3	2042	1139	0.04%	0.006%
25	3.679	800	805	809	rVB7	1750	1752	0.07%	0.009%
26	3.708	811	814	817	rBV4	1753	1175	0.04%	0.006%
27	3.923	870	881	911	rBV	180872	485261	18.51%	2.481%
28	4.074	926	928	935	rVB8	2721	1818	0.07%	0.009%
29	4.151	950	952	957	rVB5	1616	1113	0.04%	0.006%
30	4.399	1008	1029	1057	rBV	434011	1079322	41.18%	5.519%
31	4.646	1100	1106	1107	rBV5	1150	1312	0.05%	0.007%
32	4.711	1124	1126	1128	rBV4	2038	1012	0.04%	0.005%
33	4.926	1190	1193	1195	rBV3	1859	1264	0.05%	0.006%
34	5.019	1218	1222	1224	rBV4	1696	1012	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014085.D
 Acq On : 17 Dec 2019 12:00
 Operator : SY/MD
 Sample : K6308-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.093	1226	1245	1276	rBV2	1019518	2621160	100.00%	13.404%
36	5.248	1291	1293	1299	rVB7	1873	1491	0.06%	0.008%
37	5.486	1364	1367	1370	rBV4	1973	1622	0.06%	0.008%
38	5.534	1380	1382	1385	rVB4	2121	1001	0.04%	0.005%
39	5.582	1394	1397	1404	rBV9	1556	1323	0.05%	0.007%
40	5.662	1408	1422	1448	rBV	774078	1549274	59.11%	7.923%
41	5.942	1503	1509	1513	rBV9	6424	8448	0.32%	0.043%
42	6.113	1548	1562	1581	rBV	592558	1192405	45.49%	6.098%
43	6.354	1634	1637	1640	rBV5	2661	2218	0.08%	0.011%
44	6.405	1649	1653	1656	rBV4	2410	2047	0.08%	0.010%
45	6.560	1696	1701	1703	rVV5	2225	1801	0.07%	0.009%
46	6.656	1723	1731	1732	rBV7	3722	4992	0.19%	0.026%
47	6.714	1744	1749	1753	rBV5	1557	1448	0.06%	0.007%
48	6.817	1773	1781	1783	rBV9	2499	2608	0.10%	0.013%
49	6.894	1800	1805	1806	rBV4	1875	1156	0.04%	0.006%
50	6.939	1817	1819	1823	rVB3	1874	1220	0.05%	0.006%
51	6.981	1827	1832	1833	rBV5	1616	1244	0.05%	0.006%
52	7.026	1835	1846	1868	rVV	280063	508485	19.40%	2.600%
53	7.174	1884	1892	1898	rBV8	8235	14932	0.57%	0.076%
54	7.357	1934	1949	1970	rBV	1169340	2026111	77.30%	10.361%
55	7.611	2025	2028	2033	rBV6	2378	2114	0.08%	0.011%
56	7.659	2033	2043	2061	rBV	211738	368955	14.08%	1.887%
57	7.768	2075	2077	2080	rVB4	1741	1000	0.04%	0.005%
58	8.016	2152	2154	2160	rVB6	1765	1216	0.05%	0.006%
59	8.129	2178	2189	2220	rBV	526229	1142174	43.58%	5.841%
60	8.389	2269	2270	2275	rVB4	2893	1731	0.07%	0.009%
61	8.415	2275	2278	2280	rBV4	1843	1041	0.04%	0.005%
62	8.649	2347	2351	2355	rVB5	2143	2100	0.08%	0.011%
63	8.891	2413	2426	2453	rBV	1202346	1973610	75.30%	10.093%
64	9.228	2528	2531	2534	rBV5	1705	1119	0.04%	0.006%
65	9.312	2553	2557	2562	rVB6	2114	1691	0.06%	0.009%
66	9.350	2562	2569	2571	rBV6	2677	2682	0.10%	0.014%
67	9.473	2603	2607	2609	rBV4	2055	1199	0.05%	0.006%
68	9.575	2633	2639	2640	rBV3	2500	2166	0.08%	0.011%
69	9.646	2658	2661	2667	rBV7	1133	1068	0.04%	0.005%
70	9.682	2667	2672	2674	rVB5	1665	1469	0.06%	0.008%
71	9.823	2713	2716	2719	rVB4	1919	1185	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014085.D
 Acq On : 17 Dec 2019 12:00
 Operator : SY/MD
 Sample : K6308-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.849	2719	2724	2728	rBV7	1966	1928	0.07%	0.010%
73	9.881	2732	2734	2739	rVV6	1751	1382	0.05%	0.007%
74	9.971	2758	2762	2766	rVB7	1965	1560	0.06%	0.008%
75	10.254	2836	2850	2868	rBV	799109	1277050	48.72%	6.531%
76	10.421	2896	2902	2909	rBV9	4975	7851	0.30%	0.040%
77	10.476	2917	2919	2920	rBV2	2383	1099	0.04%	0.006%
78	10.881	3042	3045	3048	rBV5	2708	2798	0.11%	0.014%
79	11.100	3108	3113	3115	rBV4	2628	2151	0.08%	0.011%
80	11.128	3120	3122	3126	rVB5	2034	1335	0.05%	0.007%
81	11.193	3137	3142	3145	rBV6	2257	2256	0.09%	0.012%
82	11.289	3160	3172	3197	rBV	1045819	1624898	61.99%	8.309%
83	11.572	3251	3260	3265	rBV	5486	8391	0.32%	0.043%
84	11.665	3277	3289	3311	rBV	1104548	1750090	66.77%	8.950%
85	11.839	3340	3343	3346	rVB5	3140	1630	0.06%	0.008%
86	12.263	3474	3475	3481	rVB5	1968	1185	0.05%	0.006%
87	12.292	3481	3484	3489	rBV6	1819	1540	0.06%	0.008%
88	12.456	3531	3535	3538	rBV7	1751	1439	0.05%	0.007%
89	12.878	3663	3666	3668	rBV4	1948	1399	0.05%	0.007%
90	13.122	3740	3742	3744	rBV3	1835	1068	0.04%	0.005%
91	13.235	3772	3777	3780	rBV7	2295	2274	0.09%	0.012%
92	13.308	3790	3800	3812	rBV7	5649	10307	0.39%	0.053%
93	13.514	3860	3864	3867	rBV6	2215	1411	0.05%	0.007%
94	13.694	3918	3920	3925	rVB4	2012	1539	0.06%	0.008%
95	13.746	3934	3936	3939	rVB2	2023	1181	0.05%	0.006%
96	14.604	4201	4203	4208	rVB6	1799	1532	0.06%	0.008%
97	14.694	4229	4231	4236	rBV5	1813	1005	0.04%	0.005%
98	14.868	4280	4285	4287	rBV5	3588	2788	0.11%	0.014%
99	15.074	4346	4349	4353	rBV4	2035	1624	0.06%	0.008%
100	15.347	4431	4434	4435	rBV3	2057	1137	0.04%	0.006%


Sum of corrected areas: 19555153

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014085.D
Acq On : 17 Dec 2019 12:00
Operator : SY/MD
Sample : K6308-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

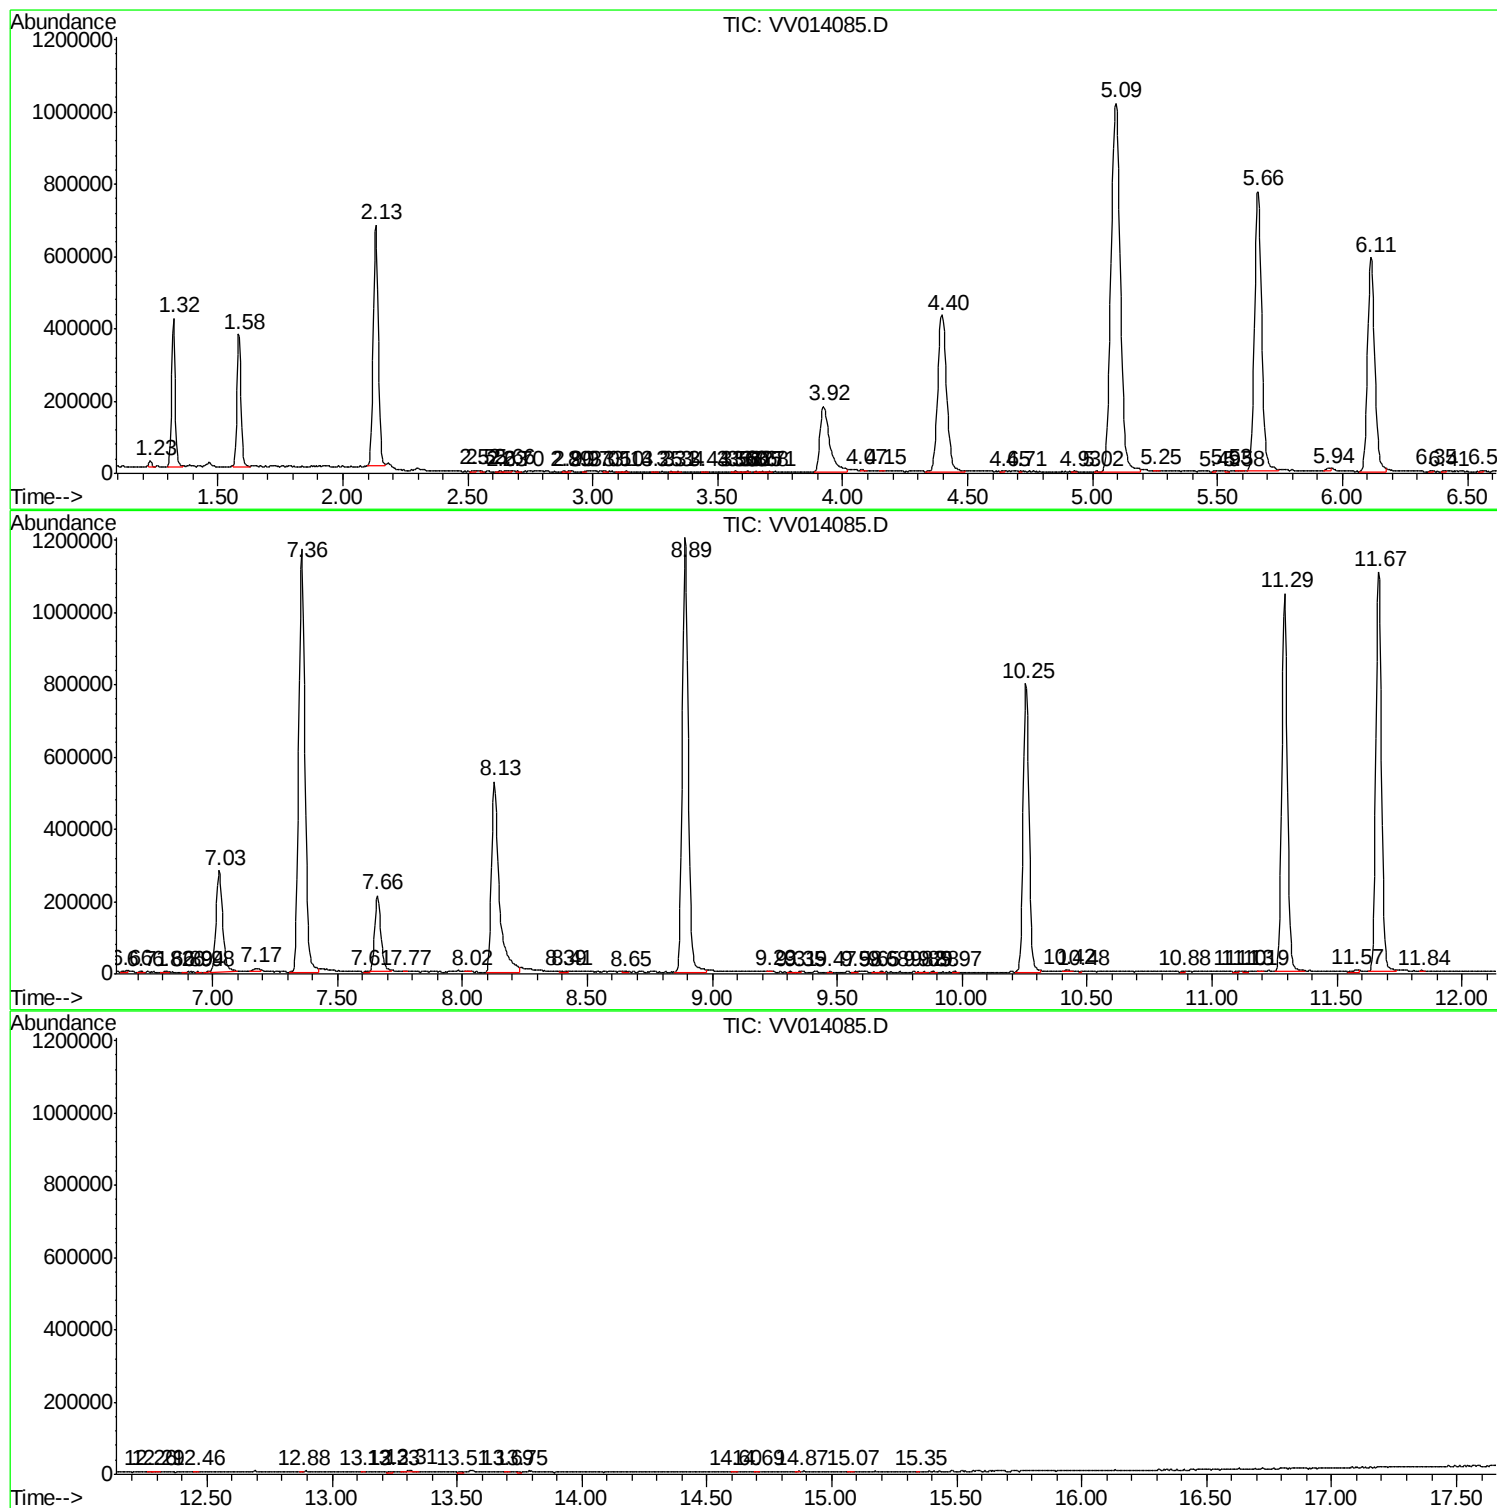

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121719\
Data File : VV014085.D
Acq On : 17 Dec 2019 12:00
Operator : SY/MD
Sample : K6308-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0C75

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014085.D
Acq On : 17 Dec 2019 12:00
Operator : SY/MD
Sample : K6308-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C75

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc