

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014086.D
 Acq On : 17 Dec 2019 12:24
 Operator : SY/MD
 Sample : K6308-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	83	rBV	395000	399401	15.39%	2.053%
2	1.582	146	153	169	rVB	368029	404709	15.59%	2.080%
3	2.129	313	323	340	rVB	665424	948038	36.52%	4.873%
4	2.396	402	406	410	rVB6	1594	1482	0.06%	0.008%
5	2.470	424	429	432	rBV7	932	1054	0.04%	0.005%
6	2.634	477	480	483	rBV4	2290	1766	0.07%	0.009%
7	2.817	535	537	543	rVB6	2462	2039	0.08%	0.010%
8	2.846	543	546	549	rBV3	1951	1305	0.05%	0.007%
9	2.871	549	554	558	rBV7	2210	1980	0.08%	0.010%
10	2.894	559	561	565	rVB4	1501	1047	0.04%	0.005%
11	2.920	565	569	573	rBV7	1253	1271	0.05%	0.007%
12	2.939	573	575	579	rVB5	2397	1680	0.06%	0.009%
13	2.968	579	584	585	rBV5	1870	1306	0.05%	0.007%
14	3.113	626	629	633	rVB5	2212	1331	0.05%	0.007%
15	3.145	636	639	641	rBV3	2071	1335	0.05%	0.007%
16	3.199	652	656	659	rVB5	1382	1191	0.05%	0.006%
17	3.415	722	723	728	rVB4	1910	1141	0.04%	0.006%
18	3.511	750	753	757	rVV6	1521	1078	0.04%	0.006%
19	3.669	797	802	806	rBV8	1127	1284	0.05%	0.007%
20	3.756	820	829	831	rBV9	2097	2264	0.09%	0.012%
21	3.865	859	863	864	rBV4	1622	1116	0.04%	0.006%
22	3.920	869	880	905	rBV	185150	479717	18.48%	2.466%
23	4.141	947	949	955	rVB7	2211	1400	0.05%	0.007%
24	4.396	1010	1028	1057	rBV2	445856	1062587	40.93%	5.462%
25	4.630	1096	1101	1103	rBV3	1730	1338	0.05%	0.007%
26	4.836	1161	1165	1169	rVB7	1733	1576	0.06%	0.008%
27	4.859	1169	1172	1175	rBV5	1879	1115	0.04%	0.006%
28	4.878	1175	1178	1181	rVB4	2043	1414	0.05%	0.007%
29	5.093	1226	1245	1278	rBV2	1013712	2596004	100.00%	13.344%
30	5.318	1312	1315	1320	rBV6	1488	1569	0.06%	0.008%
31	5.524	1377	1379	1383	rVB4	2293	1395	0.05%	0.007%
32	5.572	1392	1394	1397	rBV2	2062	1379	0.05%	0.007%
33	5.659	1408	1421	1447	rBV	819526	1639396	63.15%	8.427%
34	5.868	1483	1486	1487	rBV3	2239	1157	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014086.D
 Acq On : 17 Dec 2019 12:24
 Operator : SY/MD
 Sample : K6308-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.948	1505	1511	1521	rVB9	8077	12794	0.49%	0.066%
36	6.016	1530	1532	1535	rBV4	2056	1256	0.05%	0.006%
37	6.039	1537	1539	1541	rVV3	1817	1046	0.04%	0.005%
38	6.112	1545	1562	1588	rBV	578004	1174275	45.23%	6.036%
39	6.373	1641	1643	1647	rBV5	1688	1164	0.04%	0.006%
40	6.502	1679	1683	1685	rBV5	2408	1477	0.06%	0.008%
41	6.521	1687	1689	1694	rBV6	1712	1080	0.04%	0.006%
42	6.611	1714	1717	1720	rBV4	2245	1371	0.05%	0.007%
43	6.643	1721	1727	1730	rBV6	4781	4832	0.19%	0.025%
44	6.823	1780	1783	1790	rVB10	1824	1417	0.05%	0.007%
45	6.858	1790	1794	1796	rVB4	2065	1234	0.05%	0.006%
46	6.884	1796	1802	1803	rBV4	1731	1243	0.05%	0.006%
47	6.903	1807	1808	1811	rVB3	2571	1127	0.04%	0.006%
48	6.923	1811	1814	1818	rBV4	1720	1132	0.04%	0.006%
49	6.942	1818	1820	1821	rBV2	2260	1031	0.04%	0.005%
50	6.952	1821	1823	1830	rVB7	1719	1867	0.07%	0.010%
51	6.987	1830	1834	1835	rBV4	1877	1214	0.05%	0.006%
52	7.026	1835	1846	1862	rBV	276478	485851	18.72%	2.497%
53	7.167	1887	1890	1891	rBV3	2114	1223	0.05%	0.006%
54	7.289	1926	1928	1933	rVB5	2161	1114	0.04%	0.006%
55	7.357	1935	1949	1969	rBV	1118309	1937160	74.62%	9.958%
56	7.588	2018	2021	2024	rVB5	2356	1523	0.06%	0.008%
57	7.659	2033	2043	2060	rBV	202453	347502	13.39%	1.786%
58	7.852	2101	2103	2111	rVB8	1326	1416	0.05%	0.007%
59	8.125	2176	2188	2232	rBV	524893	1177010	45.34%	6.050%
60	8.424	2279	2281	2285	rVB4	2900	1458	0.06%	0.007%
61	8.653	2350	2352	2355	rVB4	1909	1063	0.04%	0.005%
62	8.781	2387	2392	2395	rBV6	1949	2011	0.08%	0.010%
63	8.890	2413	2426	2447	rBV	1256300	2022634	77.91%	10.397%
64	9.209	2522	2525	2532	rBV9	1605	1967	0.08%	0.010%
65	9.556	2629	2633	2638	rVB8	1597	1568	0.06%	0.008%
66	9.591	2638	2644	2647	rBV7	2386	2604	0.10%	0.013%
67	9.611	2647	2650	2655	rVB6	2118	1898	0.07%	0.010%
68	9.656	2660	2664	2665	rBV3	1566	1080	0.04%	0.006%
69	9.842	2720	2722	2726	rVV3	1823	1113	0.04%	0.006%
70	9.865	2726	2729	2732	rVV4	1909	1268	0.05%	0.007%
71	10.009	2772	2774	2779	rVB5	2164	1293	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014086.D
 Acq On : 17 Dec 2019 12:24
 Operator : SY/MD
 Sample : K6308-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.099	2794	2802	2804	rBV8	1636	1772	0.07%	0.009%
73	10.116	2804	2807	2810	rBV3	2325	1674	0.06%	0.009%
74	10.254	2836	2850	2867	rBV	770247	1242779	47.87%	6.388%
75	10.418	2897	2901	2908	rVB8	4007	4087	0.16%	0.021%
76	10.469	2913	2917	2919	rBV4	1541	1157	0.04%	0.006%
77	10.482	2919	2921	2927	rVB6	2118	1303	0.05%	0.007%
78	10.582	2950	2952	2956	rVB4	1704	1211	0.05%	0.006%
79	10.894	3046	3049	3056	rVB8	2293	2232	0.09%	0.011%
80	10.929	3058	3060	3064	rVB4	2171	1459	0.06%	0.007%
81	11.289	3160	3172	3189	rBV	1080041	1670614	64.35%	8.588%
82	11.665	3277	3289	3308	rBV	1093544	1727853	66.56%	8.882%
83	11.945	3374	3376	3381	rVB5	2071	1348	0.05%	0.007%
84	12.083	3415	3419	3420	rBV4	1766	1231	0.05%	0.006%
85	12.402	3515	3518	3520	rVB3	2356	1155	0.04%	0.006%
86	12.443	3529	3531	3537	rVB6	2059	1982	0.08%	0.010%
87	12.652	3594	3596	3601	rBV5	1785	1459	0.06%	0.007%
88	12.768	3629	3632	3634	rBV4	2420	1452	0.06%	0.007%
89	13.247	3779	3781	3785	rVB5	2165	1079	0.04%	0.006%
90	13.299	3790	3797	3799	rBV7	4146	4920	0.19%	0.025%
91	13.553	3874	3876	3878	rBV3	1884	1031	0.04%	0.005%
92	13.775	3943	3945	3947	rBV2	1959	1082	0.04%	0.006%
93	13.791	3948	3950	3952	rBV3	1931	1127	0.04%	0.006%
94	14.016	4018	4020	4025	rVB5	1732	1195	0.05%	0.006%
95	14.160	4060	4065	4069	rVB7	2262	1789	0.07%	0.009%
96	14.459	4155	4158	4163	rBV6	1245	1403	0.05%	0.007%
97	14.562	4187	4190	4192	rBV3	1556	1074	0.04%	0.006%
98	14.717	4236	4238	4242	rVB5	2110	1322	0.05%	0.007%
99	14.955	4308	4312	4315	rBV5	2174	1847	0.07%	0.009%
100	15.684	4537	4539	4540	rBV2	2231	1061	0.04%	0.005%


Sum of corrected areas: 19453879

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014086.D
Acq On : 17 Dec 2019 12:24
Operator : SY/MD
Sample : K6308-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

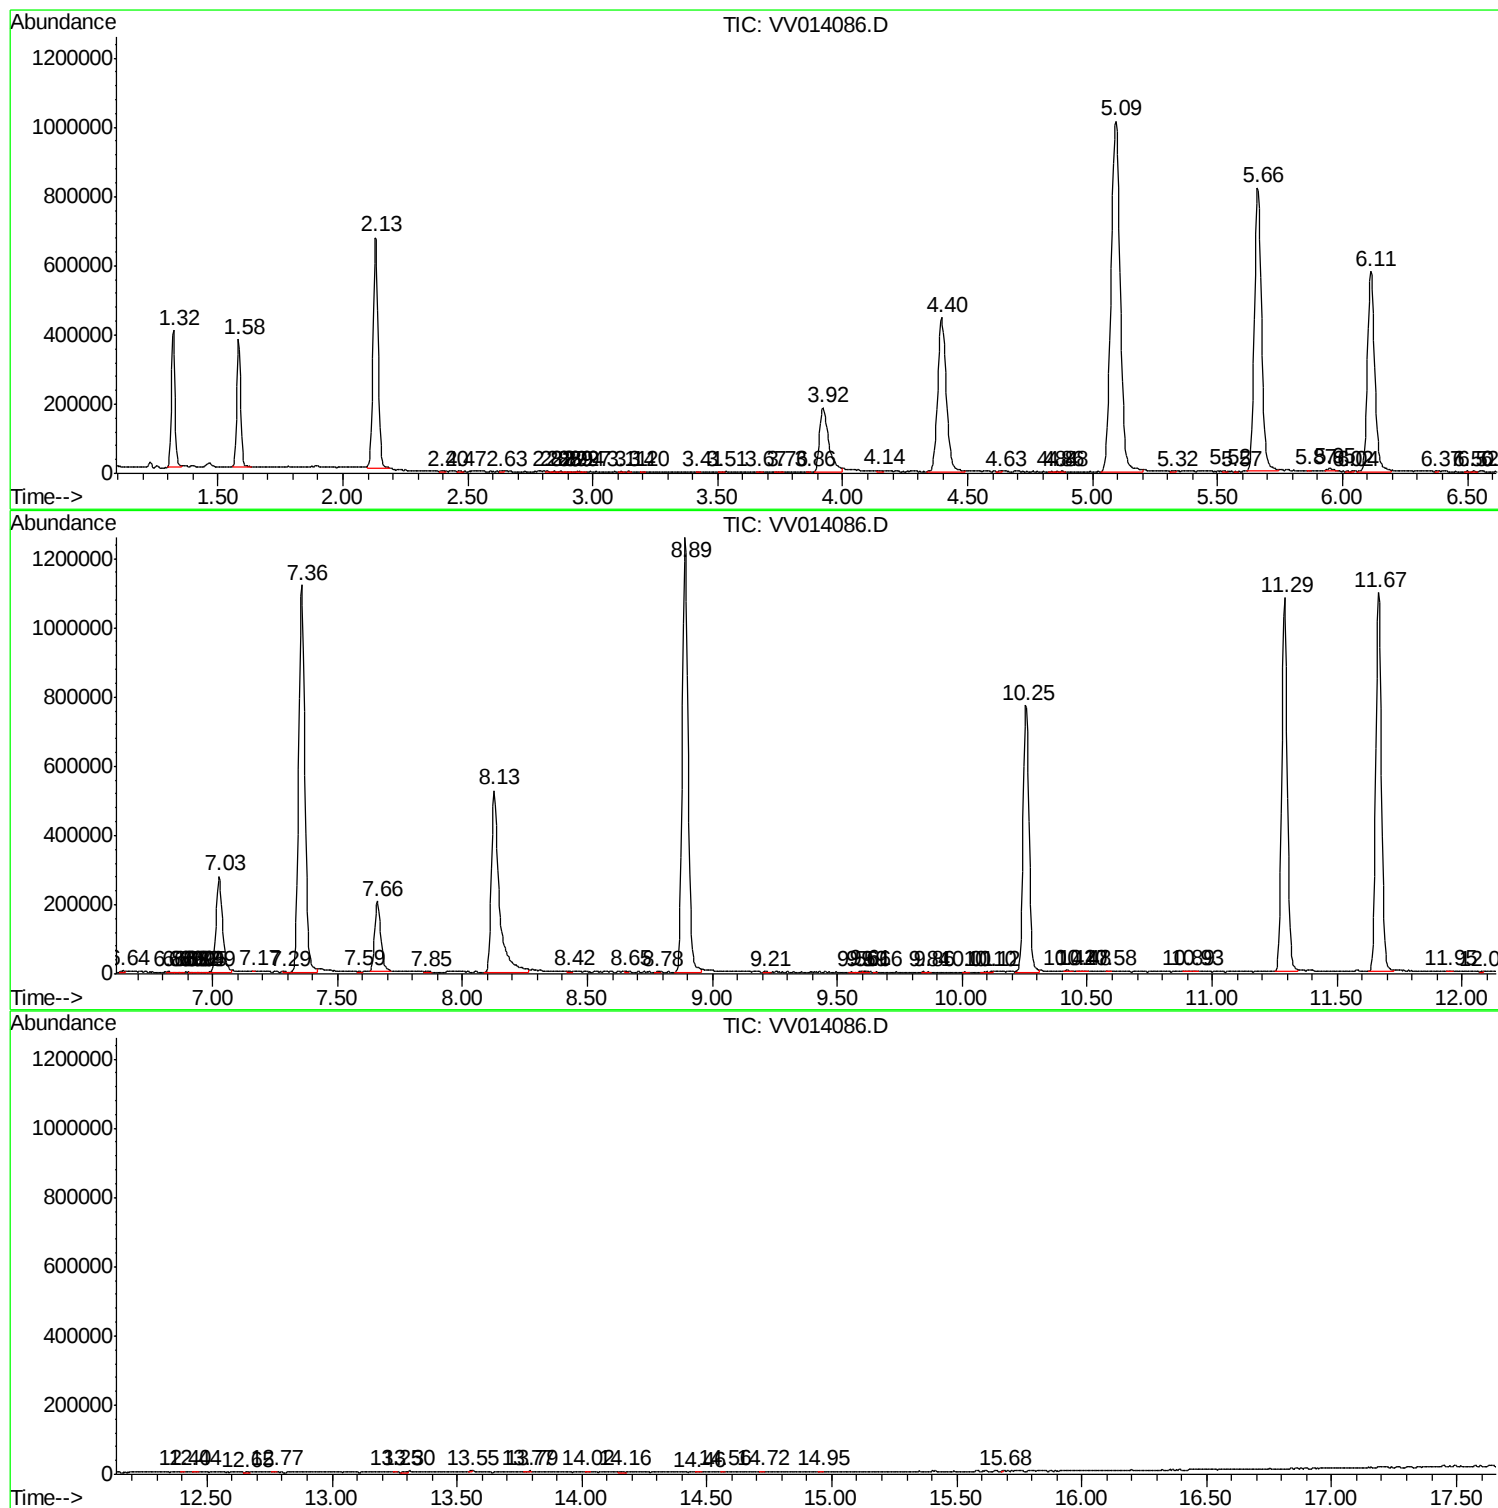

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014086.D
Acq On : 17 Dec 2019 12:24
Operator : SY/MD
Sample : K6308-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121719\
Data File : VV014086.D
Acq On : 17 Dec 2019 12:24
Operator : SY/MD
Sample : K6308-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0C82

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc