

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014087.D
 Acq On : 17 Dec 2019 12:48
 Operator : SY/MD
 Sample : K6314-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	85	rVB	392288	397644	15.77%	2.088%
2	1.582	146	153	166	rVB	349953	390098	15.47%	2.049%
3	2.129	315	323	348	rVB	636356	952182	37.76%	5.001%
4	2.727	507	509	511	rBV3	1401	515	0.02%	0.003%
5	2.778	522	525	530	rBV6	2229	2316	0.09%	0.012%
6	2.865	551	552	553	rBV	1185	326	0.01%	0.002%
7	2.875	553	555	557	rVV3	1266	658	0.03%	0.003%
8	2.904	562	564	566	rVV3	1044	605	0.02%	0.003%
9	2.926	569	571	578	rVB8	2184	2195	0.09%	0.012%
10	2.952	578	579	580	rBV	545	120	0.00%	0.001%
11	2.974	583	586	588	rBV4	2015	1431	0.06%	0.008%
12	3.045	606	608	610	rBV3	1509	628	0.02%	0.003%
13	3.103	621	626	630	rBV8	1495	1897	0.08%	0.010%
14	3.171	645	647	649	rBV3	1311	769	0.03%	0.004%
15	3.196	653	655	657	rBV4	1135	478	0.02%	0.003%
16	3.209	657	659	660	rBV2	819	311	0.01%	0.002%
17	3.257	671	674	677	rBV4	1075	971	0.04%	0.005%
18	3.280	679	681	685	rVB4	2029	1077	0.04%	0.006%
19	3.302	685	688	691	rBV3	1449	1187	0.05%	0.006%
20	3.338	696	699	702	rBV5	1598	952	0.04%	0.005%
21	3.367	706	708	709	rVV2	787	258	0.01%	0.001%
22	3.380	709	712	717	rVB6	1755	1516	0.06%	0.008%
23	3.405	717	720	723	rBV4	1980	1263	0.05%	0.007%
24	3.444	730	732	734	rBV2	557	259	0.01%	0.001%
25	3.460	734	737	742	rVB6	1942	1582	0.06%	0.008%
26	3.486	742	745	746	rBV3	639	289	0.01%	0.002%
27	3.598	775	780	783	rBV6	1453	1364	0.05%	0.007%
28	3.614	783	785	790	rVB4	1628	1001	0.04%	0.005%
29	3.640	790	793	794	rBV3	932	557	0.02%	0.003%
30	3.666	800	801	803	rBV2	1735	471	0.02%	0.002%
31	3.695	807	810	811	rVB3	780	274	0.01%	0.001%
32	3.704	811	813	815	rBV3	1051	592	0.02%	0.003%
33	3.727	818	820	822	rBV3	1278	483	0.02%	0.003%
34	3.817	843	848	849	rBV4	738	489	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014087.D
 Acq On : 17 Dec 2019 12:48
 Operator : SY/MD
 Sample : K6314-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	3.865	856	863	865	rBV7	1769	1731	0.07%	0.009%
36	3.923	869	881	908	rBV	178034	475684	18.86%	2.498%
37	4.399	1013	1029	1051	rBV	419638	1026100	40.69%	5.389%
38	4.756	1138	1140	1143	rVB4	2365	996	0.04%	0.005%
39	4.775	1143	1146	1150	rBV5	2382	1773	0.07%	0.009%
40	4.830	1160	1163	1165	rVB3	1245	527	0.02%	0.003%
41	4.875	1175	1177	1179	rBV3	951	384	0.02%	0.002%
42	5.093	1226	1245	1268	rBV2	997214	2521761	100.00%	13.244%
43	5.659	1408	1421	1444	rBV	794307	1580888	62.69%	8.302%
44	6.113	1549	1562	1586	rBV	549584	1120794	44.44%	5.886%
45	6.531	1690	1692	1695	rBV3	1270	664	0.03%	0.003%
46	6.547	1695	1697	1700	rBV4	1638	1176	0.05%	0.006%
47	6.634	1721	1724	1725	rBV3	1749	979	0.04%	0.005%
48	6.884	1801	1802	1806	rBV4	967	487	0.02%	0.003%
49	6.907	1806	1809	1811	rVB3	972	584	0.02%	0.003%
50	6.916	1811	1812	1814	rBV2	787	371	0.01%	0.002%
51	6.965	1824	1827	1829	rBV5	1124	758	0.03%	0.004%
52	6.981	1829	1832	1833	rBV3	1411	823	0.03%	0.004%
53	7.026	1835	1846	1869	rVV	259981	475892	18.87%	2.499%
54	7.357	1935	1949	1968	rBV	1094484	1890072	74.95%	9.926%
55	7.659	2033	2043	2067	rBV	200857	351047	13.92%	1.844%
56	7.891	2113	2115	2117	rBV3	2434	1582	0.06%	0.008%
57	8.129	2177	2189	2226	rBV	531006	1132815	44.92%	5.949%
58	8.489	2298	2301	2305	rVB6	1930	938	0.04%	0.005%
59	8.891	2413	2426	2450	rBV	1227802	2005145	79.51%	10.531%
60	9.158	2507	2509	2512	rBV3	1869	1197	0.05%	0.006%
61	9.257	2538	2540	2542	rBV3	1604	679	0.03%	0.004%
62	9.325	2559	2561	2562	rBV2	1480	505	0.02%	0.003%
63	9.421	2588	2591	2592	rBV3	1072	613	0.02%	0.003%
64	9.498	2613	2615	2618	rBV4	934	436	0.02%	0.002%
65	9.514	2618	2620	2622	rBV2	1142	575	0.02%	0.003%
66	9.537	2625	2627	2629	rBV2	1973	865	0.03%	0.005%
67	9.595	2637	2645	2646	rBV7	4411	3948	0.16%	0.021%
68	9.653	2662	2663	2665	rBV2	1245	679	0.03%	0.004%
69	9.768	2697	2699	2701	rBV3	1522	897	0.04%	0.005%
70	10.045	2784	2785	2786	rBV	890	229	0.01%	0.001%
71	10.064	2789	2791	2794	rBV3	1166	631	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014087.D
Acq On : 17 Dec 2019 12:48
Operator : SY/MD
Sample : K6314-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF22

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	10.103	2797	2803	2805	rBV5	1559	1435	0.06%	0.008%
73	10.154	2814	2819	2823	rBV7	2586	3097	0.12%	0.016%
74	10.254	2839	2850	2868	rBV	768753	1202082	47.67%	6.313%
75	11.061	3098	3101	3106	rBV5	2388	2192	0.09%	0.012%
76	11.289	3160	3172	3191	rBV	1117879	1721177	68.25%	9.039%
77	11.665	3278	3289	3307	rBV	1105944	1735503	68.82%	9.114%
78	12.363	3505	3506	3509	rBV3	2106	1255	0.05%	0.007%
79	12.572	3568	3571	3574	rBV5	1485	928	0.04%	0.005%
80	13.466	3845	3849	3851	rBV4	2108	1653	0.07%	0.009%




Sum of corrected areas: 19041305

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014087.D
Acq On : 17 Dec 2019 12:48
Operator : SY/MD
Sample : K6314-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

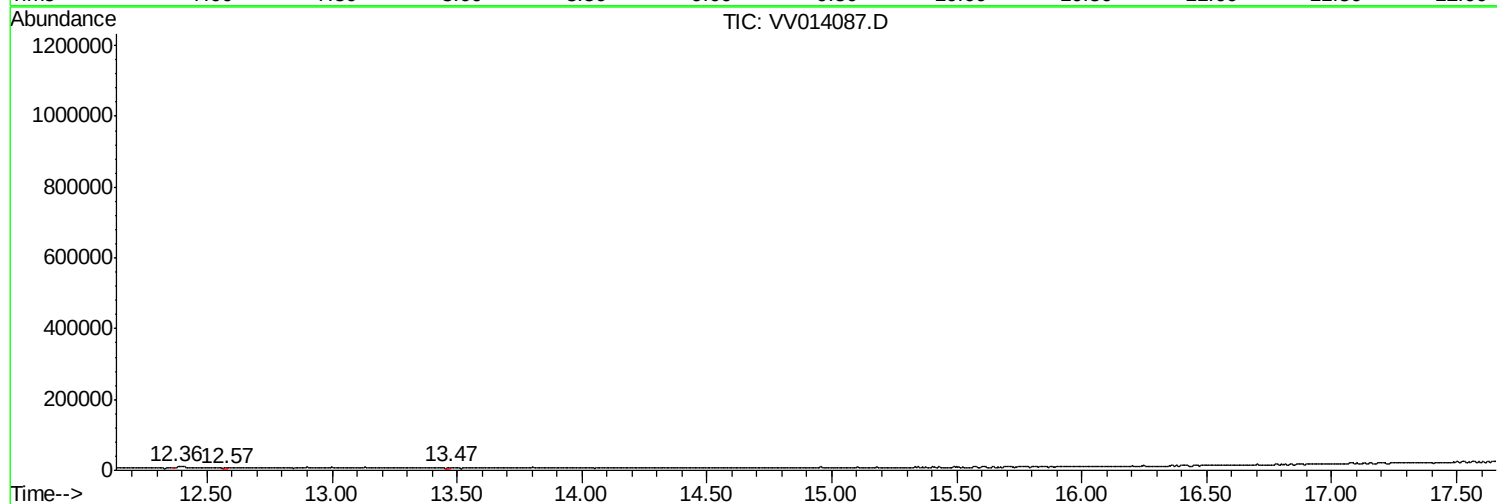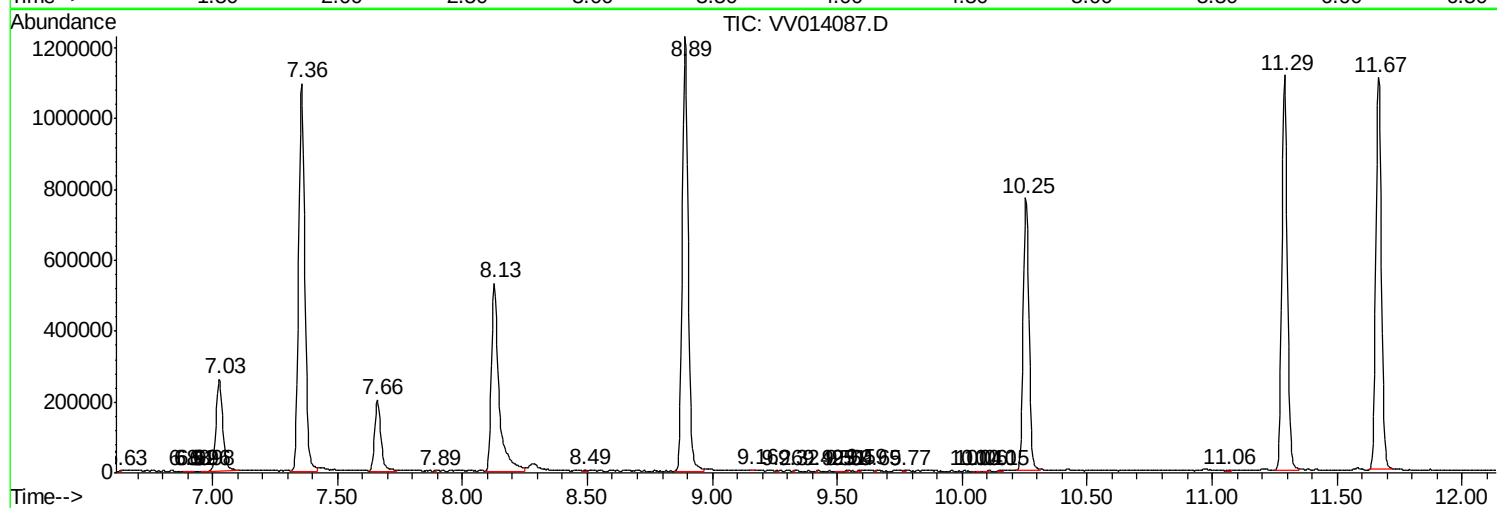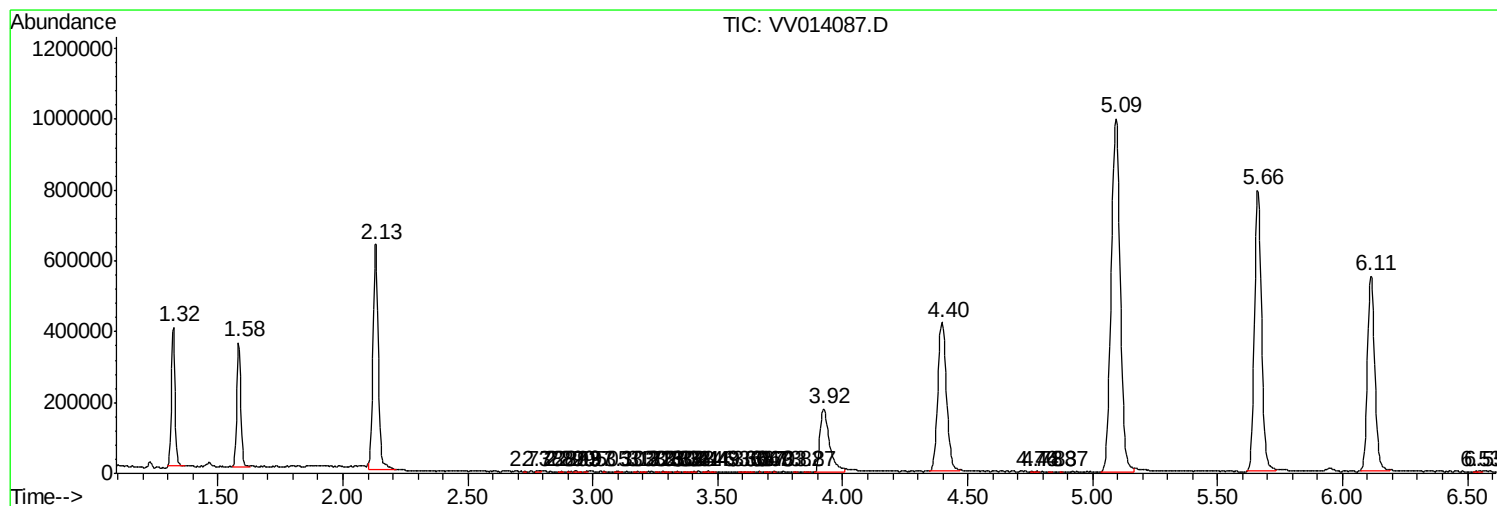

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014087.D
Acq On : 17 Dec 2019 12:48
Operator : SY/MD
Sample : K6314-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121719\
Data File : VV014087.D
Acq On : 17 Dec 2019 12:48
Operator : SY/MD
Sample : K6314-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFF22

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc