

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014090.D
 Acq On : 17 Dec 2019 13:59
 Operator : SY/MD
 Sample : K6280-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	39	43	48	rVB2	19872	16848	0.68%	0.090%
2	1.322	64	72	83	rBV	381835	387668	15.69%	2.077%
3	1.582	145	153	165	rVB	338822	381262	15.43%	2.043%
4	2.129	314	323	335	rBV	621673	863791	34.96%	4.628%
5	2.386	398	403	405	rBV5	2779	2638	0.11%	0.014%
6	2.463	425	427	431	rVV4	1596	1084	0.04%	0.006%
7	2.769	518	522	523	rBV3	1451	1145	0.05%	0.006%
8	2.782	523	526	529	rVV5	1858	1210	0.05%	0.006%
9	2.965	581	583	588	rVB6	1519	1162	0.05%	0.006%
10	3.174	642	648	650	rBV7	1571	1881	0.08%	0.010%
11	3.225	662	664	668	rVB5	1544	1015	0.04%	0.005%
12	3.293	679	685	688	rVB7	1747	1676	0.07%	0.009%
13	3.328	691	696	701	rBV7	1457	1320	0.05%	0.007%
14	3.367	703	708	710	rBV4	2369	1513	0.06%	0.008%
15	3.421	721	725	729	rVB6	1292	1032	0.04%	0.006%
16	3.454	732	735	737	rBV3	2036	1223	0.05%	0.007%
17	3.534	757	760	765	rBV6	1655	1525	0.06%	0.008%
18	3.614	782	785	791	rVB7	1893	1691	0.07%	0.009%
19	3.675	800	804	809	rVB8	1899	2289	0.09%	0.012%
20	3.701	809	812	815	rBV5	1684	1372	0.06%	0.007%
21	3.791	836	840	842	rBV4	1225	1055	0.04%	0.006%
22	3.855	856	860	863	rBV5	2327	1616	0.07%	0.009%
23	3.923	869	881	908	rBV2	182200	479977	19.42%	2.571%
24	4.232	975	977	980	rVB4	2078	1168	0.05%	0.006%
25	4.396	1009	1028	1053	rBV	422971	1018270	41.21%	5.455%
26	4.730	1130	1132	1134	rVB3	2184	1027	0.04%	0.006%
27	4.830	1158	1163	1166	rBV7	2222	1953	0.08%	0.010%
28	4.942	1196	1198	1200	rBV3	1987	1108	0.04%	0.006%
29	5.093	1227	1245	1273	rBV2	986887	2471104	100.00%	13.238%
30	5.344	1319	1323	1325	rBV4	1462	1285	0.05%	0.007%
31	5.379	1332	1334	1338	rVB4	2090	1185	0.05%	0.006%
32	5.659	1408	1421	1452	rVV	806033	1599023	64.71%	8.566%
33	5.945	1502	1510	1515	rBV7	8076	12793	0.52%	0.069%
34	5.984	1520	1522	1525	rVV4	1965	1086	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014090.D
 Acq On : 17 Dec 2019 13:59
 Operator : SY/MD
 Sample : K6280-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.035	1536	1538	1542	rBV5	1349	1050	0.04%	0.006%
36	6.113	1548	1562	1590	rBV	556897	1130227	45.74%	6.055%
37	6.482	1674	1677	1680	rVB4	3120	1744	0.07%	0.009%
38	6.505	1680	1684	1687	rVB5	1700	1459	0.06%	0.008%
39	6.543	1691	1696	1697	rBV5	2422	1617	0.07%	0.009%
40	6.585	1704	1709	1713	rBV7	1857	1707	0.07%	0.009%
41	6.614	1713	1718	1719	rBV2	1720	1239	0.05%	0.007%
42	6.801	1770	1776	1780	rBV9	2018	2414	0.10%	0.013%
43	6.894	1802	1805	1809	rBV6	1514	1017	0.04%	0.005%
44	7.026	1834	1846	1864	rBV	260853	464485	18.80%	2.488%
45	7.154	1883	1886	1887	rBV3	2062	1303	0.05%	0.007%
46	7.357	1934	1949	1967	rBV	1045582	1812240	73.34%	9.709%
47	7.576	2015	2017	2021	rVB4	1652	1045	0.04%	0.006%
48	7.614	2026	2029	2031	rBV3	1828	1246	0.05%	0.007%
49	7.659	2033	2043	2061	rBV	191399	324697	13.14%	1.739%
50	7.810	2087	2090	2093	rBV4	1382	1102	0.04%	0.006%
51	7.823	2093	2094	2098	rVV4	1800	1067	0.04%	0.006%
52	7.842	2098	2100	2107	rVV7	1562	1112	0.05%	0.006%
53	8.010	2148	2152	2155	rVB5	2173	1641	0.07%	0.009%
54	8.055	2161	2166	2169	rBV7	1749	1501	0.06%	0.008%
55	8.125	2178	2188	2219	rBV	527670	1080195	43.71%	5.787%
56	8.466	2291	2294	2297	rVB4	2619	1549	0.06%	0.008%
57	8.637	2345	2347	2349	rBV3	2333	1126	0.05%	0.006%
58	8.891	2412	2426	2448	rBV	1177487	1908387	77.23%	10.224%
59	9.206	2522	2524	2529	rVB4	2227	1272	0.05%	0.007%
60	9.286	2545	2549	2553	rVB6	1983	1180	0.05%	0.006%
61	9.479	2606	2609	2611	rBV3	1328	991	0.04%	0.005%
62	9.588	2640	2643	2646	rBV4	1950	1370	0.06%	0.007%
63	9.640	2657	2659	2663	rVB4	1593	995	0.04%	0.005%
64	9.675	2666	2670	2673	rBV6	1585	1147	0.05%	0.006%
65	9.701	2673	2678	2680	rVB5	1620	1330	0.05%	0.007%
66	9.743	2688	2691	2694	rBV3	1510	1038	0.04%	0.006%
67	9.849	2721	2724	2730	rBV6	1194	1270	0.05%	0.007%
68	9.894	2733	2738	2740	rBV6	1643	1326	0.05%	0.007%
69	9.932	2748	2750	2754	rVB4	1330	976	0.04%	0.005%
70	10.029	2776	2780	2783	rVB5	1327	1063	0.04%	0.006%
71	10.129	2808	2811	2813	rBV3	1502	1122	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014090.D
 Acq On : 17 Dec 2019 13:59
 Operator : SY/MD
 Sample : K6280-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.257	2839	2851	2870	rBV	724041	1149044	46.50%	6.156%
73	10.498	2922	2926	2929	rVB4	1579	1108	0.04%	0.006%
74	10.521	2929	2933	2934	rBV3	1997	1337	0.05%	0.007%
75	10.704	2987	2990	2991	rBV3	1613	1039	0.04%	0.006%
76	10.878	3040	3044	3046	rBV4	1869	1546	0.06%	0.008%
77	10.936	3060	3062	3065	rBV4	1869	1279	0.05%	0.007%
78	11.193	3139	3142	3145	rBV4	2906	2430	0.10%	0.013%
79	11.289	3159	3172	3193	rBV	1092902	1719162	69.57%	9.210%
80	11.501	3235	3238	3240	rBV4	1809	1045	0.04%	0.006%
81	11.579	3253	3262	3276	rBV5	14598	29333	1.19%	0.157%
82	11.665	3276	3289	3309	rBV	1085597	1698103	68.72%	9.097%
83	11.984	3384	3388	3389	rBV4	1893	1064	0.04%	0.006%
84	12.395	3509	3516	3523	rBV4	4985	6859	0.28%	0.037%
85	12.608	3580	3582	3586	rVB4	1922	1129	0.05%	0.006%
86	12.894	3669	3671	3675	rBV5	2908	2132	0.09%	0.011%
87	13.029	3711	3713	3718	rVB5	3299	2244	0.09%	0.012%
88	13.051	3718	3720	3724	rBV4	2108	1463	0.06%	0.008%
89	13.128	3738	3744	3748	rBV6	2565	3397	0.14%	0.018%
90	13.299	3793	3797	3801	rBV6	2150	2131	0.09%	0.011%
91	13.585	3883	3886	3888	rBV4	1602	1110	0.04%	0.006%
92	13.771	3941	3944	3947	rBV5	1914	1750	0.07%	0.009%
93	13.820	3957	3959	3962	rVB3	3082	1359	0.05%	0.007%
94	13.845	3962	3967	3970	rBV6	1946	1995	0.08%	0.011%
95	14.659	4216	4220	4221	rBV3	2485	1719	0.07%	0.009%
96	14.923	4298	4302	4303	rBV4	1767	1297	0.05%	0.007%
97	15.000	4324	4326	4331	rVV6	1367	1128	0.05%	0.006%
98	15.070	4345	4348	4349	rBV3	2456	1332	0.05%	0.007%
99	15.122	4361	4364	4368	rBV5	1299	1215	0.05%	0.007%
100	15.813	4576	4579	4580	rBV3	2362	1417	0.06%	0.008%


Sum of corrected areas: 18666412

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014090.D
Acq On : 17 Dec 2019 13:59
Operator : SY/MD
Sample : K6280-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BFF45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

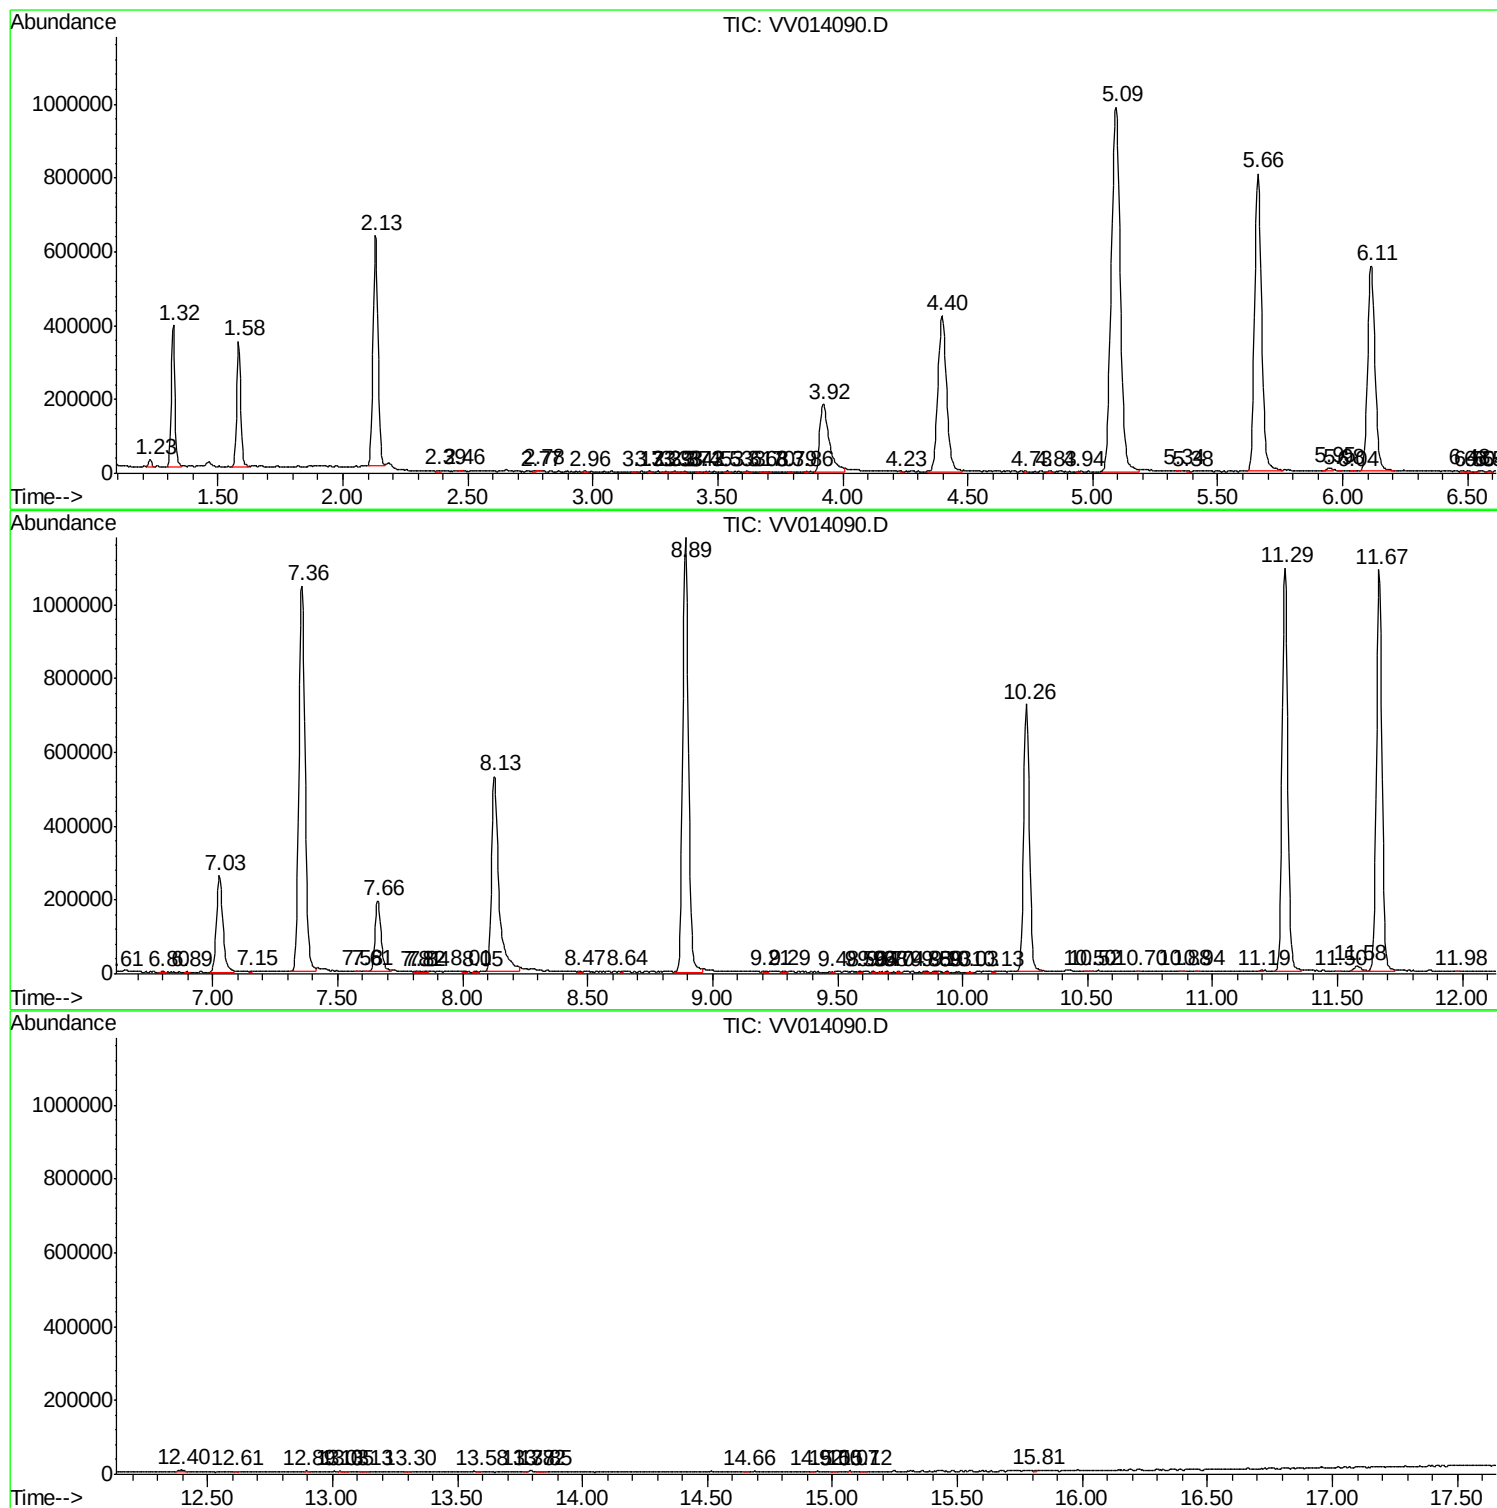

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014090.D
Acq On : 17 Dec 2019 13:59
Operator : SY/MD
Sample : K6280-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014090.D
Acq On : 17 Dec 2019 13:59
Operator : SY/MD
Sample : K6280-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF45

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc