

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014091.D
 Acq On : 17 Dec 2019 14:22
 Operator : SY/MD
 Sample : K6276-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	378832	378038	15.25%	2.044%
2	1.582	146	153	168	rVB	354778	394603	15.92%	2.133%
3	2.129	315	323	336	rVB	636739	881659	35.56%	4.766%
4	2.569	458	460	463	rBV4	1985	940	0.04%	0.005%
5	2.766	518	521	523	rBV4	2703	1908	0.08%	0.010%
6	2.901	561	563	566	rVB4	1562	600	0.02%	0.003%
7	2.968	582	584	585	rBV2	1440	415	0.02%	0.002%
8	2.991	589	591	593	rBV3	1254	548	0.02%	0.003%
9	3.004	593	595	597	rBV3	1118	758	0.03%	0.004%
10	3.155	640	642	647	rVB4	1674	999	0.04%	0.005%
11	3.187	647	652	654	rBV6	1750	1468	0.06%	0.008%
12	3.209	654	659	662	rBV7	1360	1476	0.06%	0.008%
13	3.328	694	696	697	rBV2	709	211	0.01%	0.001%
14	3.399	716	718	720	rBV3	1505	828	0.03%	0.004%
15	3.537	759	761	763	rBV3	1369	694	0.03%	0.004%
16	3.589	776	777	780	rBV2	1573	538	0.02%	0.003%
17	3.605	780	782	783	rBV2	1117	261	0.01%	0.001%
18	3.621	783	787	790	rBV4	988	885	0.04%	0.005%
19	3.672	801	803	806	rVB5	988	474	0.02%	0.003%
20	3.701	810	812	814	rBV2	1041	650	0.03%	0.004%
21	3.743	822	825	827	rBV3	1400	950	0.04%	0.005%
22	3.795	839	841	844	rVB4	1875	854	0.03%	0.005%
23	3.823	846	850	851	rBV2	1672	1226	0.05%	0.007%
24	3.852	857	859	864	rVB5	1452	849	0.03%	0.005%
25	3.872	864	865	869	rBV4	1278	960	0.04%	0.005%
26	3.920	869	880	910	rBV	183093	496694	20.03%	2.685%
27	4.396	1013	1028	1049	rBV	409507	995926	40.17%	5.384%
28	4.811	1155	1157	1158	rBV2	2013	656	0.03%	0.004%
29	4.965	1204	1205	1209	rBV3	995	749	0.03%	0.004%
30	5.023	1220	1223	1224	rBV2	1372	827	0.03%	0.004%
31	5.090	1227	1244	1278	rVV2	972068	2479211	100.00%	13.402%
32	5.659	1407	1421	1439	rBV	807434	1587477	64.03%	8.582%
33	6.052	1540	1543	1545	rBV4	2101	1445	0.06%	0.008%
34	6.113	1550	1562	1586	rVV	539189	1074415	43.34%	5.808%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014091.D
Acq On : 17 Dec 2019 14:22
Operator : SY/MD
Sample : K6276-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C73

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

35	6.650	1718	1729	1730	rBV9	5204	7054	0.28%	0.038%
36	6.753	1760	1761	1764	rVB3	1500	701	0.03%	0.004%
37	7.026	1833	1846	1869	rBV2	258908	477196	19.25%	2.580%
38	7.180	1885	1894	1902	rBV2	6931	13980	0.56%	0.076%
39	7.357	1936	1949	1967	rBV	1050584	1834749	74.01%	9.918%
40	7.659	2033	2043	2062	rBV	194563	332287	13.40%	1.796%
41	8.126	2178	2188	2231	rBV	501543	1087854	43.88%	5.881%
42	8.572	2323	2327	2329	rBV5	2491	1689	0.07%	0.009%
43	8.643	2347	2349	2351	rBV3	2202	842	0.03%	0.005%
44	8.891	2414	2426	2447	rBV	1192134	1920369	77.46%	10.381%
45	9.280	2544	2547	2549	rBV4	2133	1208	0.05%	0.007%
46	9.367	2573	2574	2577	rVB2	1763	773	0.03%	0.004%
47	9.425	2589	2592	2595	rBV5	1299	1001	0.04%	0.005%
48	9.453	2598	2601	2606	rVV6	1425	1503	0.06%	0.008%
49	9.486	2609	2611	2614	rVB4	2122	916	0.04%	0.005%
50	9.769	2697	2699	2701	rBV3	1505	592	0.02%	0.003%
51	9.971	2759	2762	2765	rBV4	2775	2068	0.08%	0.011%
52	10.016	2774	2776	2780	rVB4	1114	507	0.02%	0.003%
53	10.035	2780	2782	2786	rBV4	2381	1486	0.06%	0.008%
54	10.068	2790	2792	2795	rBV5	1501	1030	0.04%	0.006%
55	10.132	2809	2812	2813	rBV3	1708	921	0.04%	0.005%
56	10.177	2824	2826	2829	rVB5	1971	826	0.03%	0.004%
57	10.257	2839	2851	2873	rBV	707870	1150943	46.42%	6.222%
58	10.887	3044	3047	3050	rBV4	2966	2298	0.09%	0.012%
59	11.289	3160	3172	3192	rBV	1092947	1705420	68.79%	9.219%
60	11.666	3278	3289	3309	rBV	1033019	1640322	66.16%	8.867%


Sum of corrected areas: 18498727

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014091.D
Acq On : 17 Dec 2019 14:22
Operator : SY/MD
Sample : K6276-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

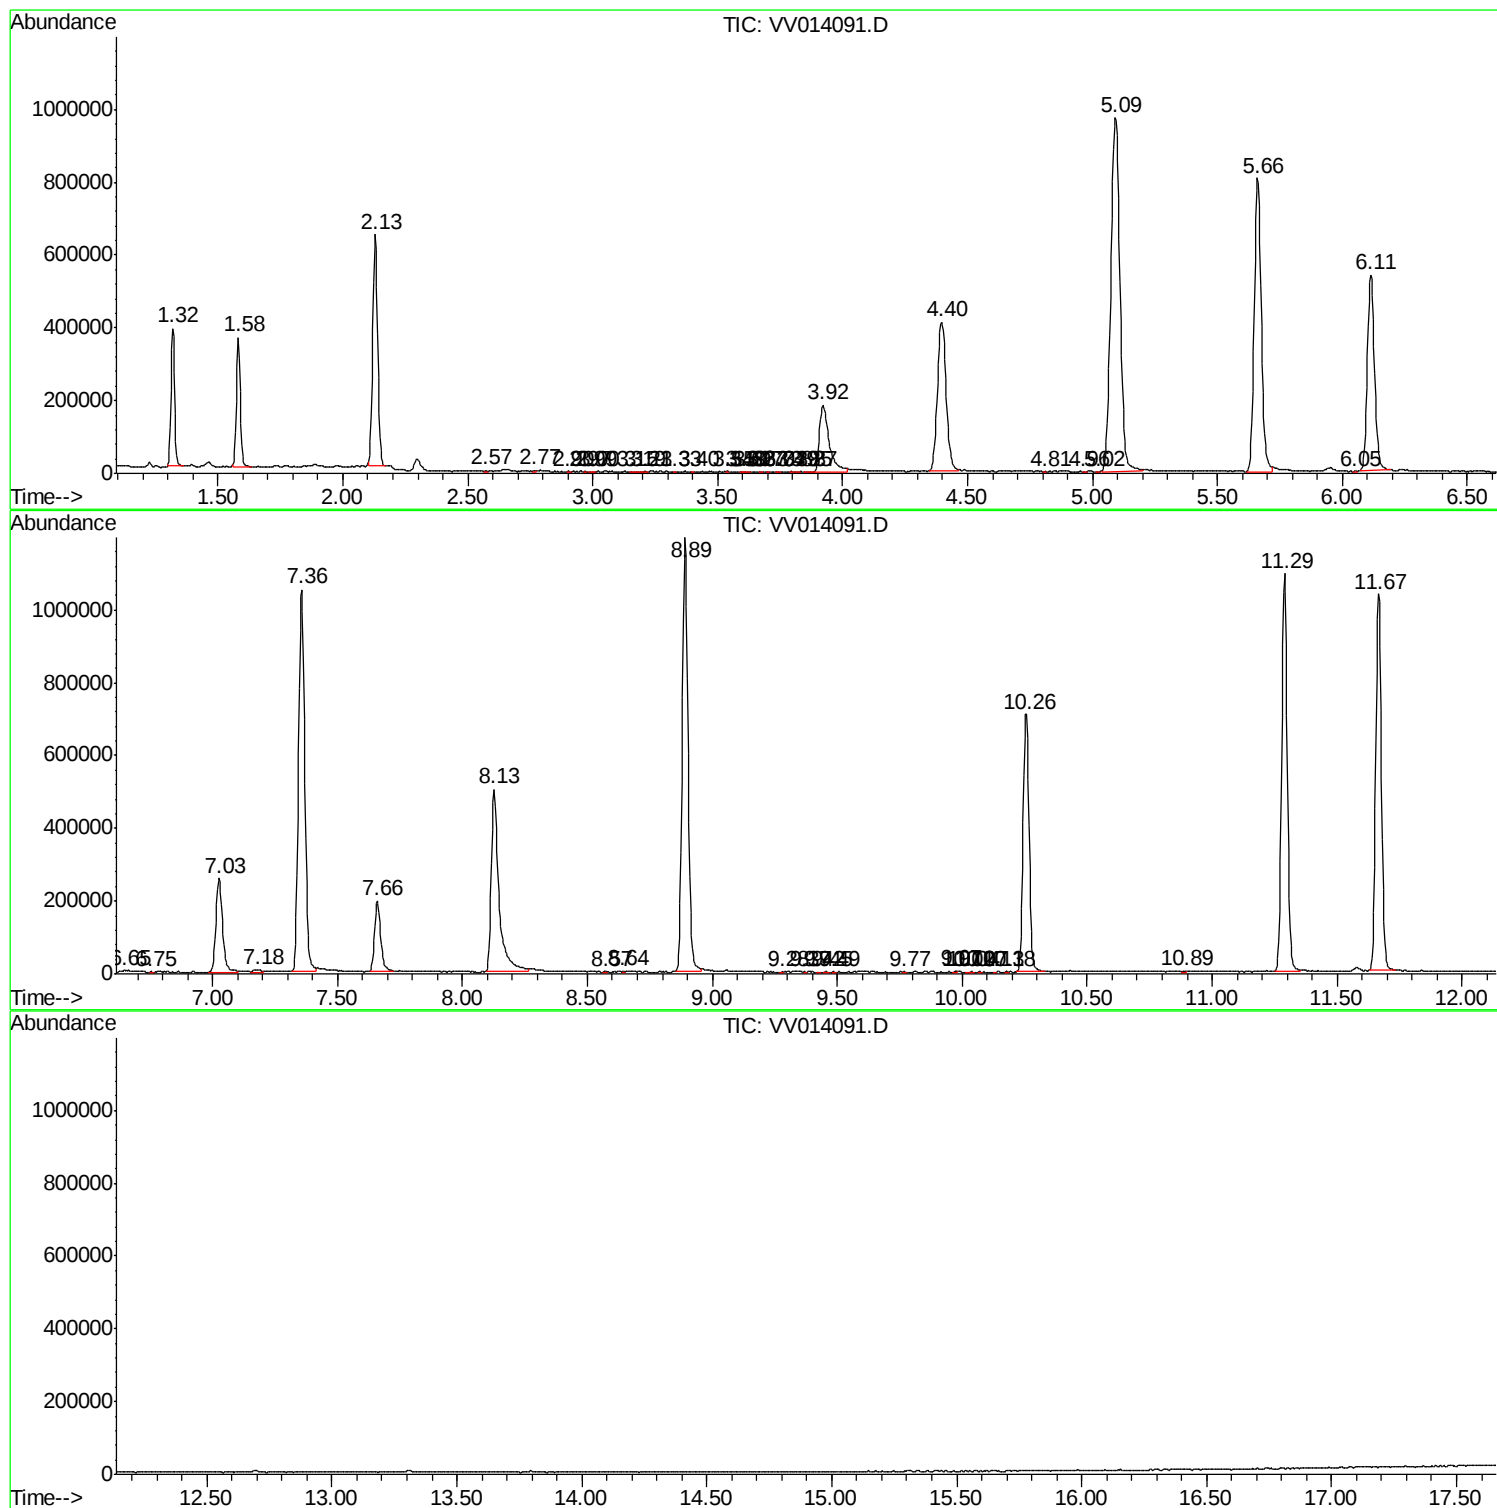

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014091.D
Acq On : 17 Dec 2019 14:22
Operator : SY/MD
Sample : K6276-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014091.D
Acq On : 17 Dec 2019 14:22
Operator : SY/MD
Sample : K6276-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc