

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014093.D
 Acq On : 17 Dec 2019 15:10
 Operator : SY/MD
 Sample : K6276-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	88	rVB	384629	390586	15.63%	2.063%
2	1.582	147	153	168	rVB	345337	384566	15.39%	2.031%
3	2.129	315	323	337	rVB	628108	893492	35.75%	4.719%
4	2.611	469	473	477	rBV6	1826	1910	0.08%	0.010%
5	2.820	537	538	542	rVB4	2132	1141	0.05%	0.006%
6	2.901	561	563	566	rBV4	1031	686	0.03%	0.004%
7	2.958	577	581	583	rBV4	2081	1641	0.07%	0.009%
8	3.013	593	598	602	rVB5	1914	1738	0.07%	0.009%
9	3.071	614	616	620	rBV4	1144	893	0.04%	0.005%
10	3.087	620	621	623	rVV2	1178	448	0.02%	0.002%
11	3.119	627	631	632	rBV4	1031	794	0.03%	0.004%
12	3.148	638	640	644	rBV3	905	638	0.03%	0.003%
13	3.206	655	658	659	rBV2	1584	697	0.03%	0.004%
14	3.228	663	665	667	rBV2	714	378	0.02%	0.002%
15	3.241	667	669	671	rBV2	1647	743	0.03%	0.004%
16	3.277	678	680	682	rBV3	931	421	0.02%	0.002%
17	3.376	709	711	714	rBV2	751	406	0.02%	0.002%
18	3.412	720	722	723	rBV2	1084	394	0.02%	0.002%
19	3.428	725	727	729	rVV3	1523	728	0.03%	0.004%
20	3.495	746	748	751	rVB3	1066	357	0.01%	0.002%
21	3.537	758	761	763	rBV4	1220	794	0.03%	0.004%
22	3.560	766	768	770	rBV3	703	357	0.01%	0.002%
23	3.598	778	780	782	rBV2	1746	824	0.03%	0.004%
24	3.627	785	789	792	rVB6	1463	1318	0.05%	0.007%
25	3.650	792	796	798	rBV4	1627	1027	0.04%	0.005%
26	3.688	804	808	809	rBV3	1425	895	0.04%	0.005%
27	3.733	818	822	825	rBV5	1303	1263	0.05%	0.007%
28	3.765	831	832	836	rVB4	975	537	0.02%	0.003%
29	3.791	836	840	843	rBV5	2262	2061	0.08%	0.011%
30	3.852	855	859	861	rBV3	1264	770	0.03%	0.004%
31	3.920	869	880	911	rBV2	186890	506473	20.27%	2.675%
32	4.286	993	994	998	rBV4	1192	610	0.02%	0.003%
33	4.338	1008	1010	1012	rBV3	1805	1023	0.04%	0.005%
34	4.399	1014	1029	1052	rVB	429232	1026327	41.07%	5.421%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014093.D
 Acq On : 17 Dec 2019 15:10
 Operator : SY/MD
 Sample : K6276-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.743	1133	1136	1137	rBV3	1598	929	0.04%	0.005%
36	4.798	1150	1153	1158	rVB7	2524	1600	0.06%	0.008%
37	4.833	1162	1164	1168	rBV4	1677	1143	0.05%	0.006%
38	4.849	1168	1169	1172	rBV3	1025	567	0.02%	0.003%
39	4.984	1208	1211	1217	rBV7	1205	1183	0.05%	0.006%
40	5.010	1217	1219	1221	rVB3	1108	508	0.02%	0.003%
41	5.023	1221	1223	1225	rBV3	1654	907	0.04%	0.005%
42	5.093	1227	1245	1274	rBV2	982787	2499138	100.00%	13.199%
43	5.531	1379	1381	1384	rBV3	1977	1268	0.05%	0.007%
44	5.582	1395	1397	1400	rBV3	2009	1558	0.06%	0.008%
45	5.659	1409	1421	1453	rBV	829968	1642244	65.71%	8.674%
46	6.000	1525	1527	1531	rVB4	1815	1091	0.04%	0.006%
47	6.113	1547	1562	1588	rBV	567647	1156491	46.28%	6.108%
48	6.505	1680	1684	1685	rBV3	1622	1075	0.04%	0.006%
49	6.650	1721	1729	1730	rBV8	3673	4329	0.17%	0.023%
50	6.752	1759	1761	1764	rBV3	1921	777	0.03%	0.004%
51	6.814	1778	1780	1781	rVB2	1739	532	0.02%	0.003%
52	6.830	1783	1785	1788	rBV4	1095	692	0.03%	0.004%
53	6.855	1788	1793	1798	rVB8	2043	1846	0.07%	0.010%
54	6.888	1800	1803	1805	rBV4	2140	1299	0.05%	0.007%
55	6.949	1820	1822	1824	rBV3	932	327	0.01%	0.002%
56	7.026	1834	1846	1865	rBV	264342	473432	18.94%	2.500%
57	7.357	1936	1949	1969	rBV	1082442	1865761	74.66%	9.854%
58	7.659	2033	2043	2065	rBV	192604	333615	13.35%	1.762%
59	7.820	2091	2093	2095	rBV3	1747	786	0.03%	0.004%
60	7.968	2138	2139	2140	rBV	1415	443	0.02%	0.002%
61	8.032	2157	2159	2166	rBV8	1887	1216	0.05%	0.006%
62	8.125	2177	2188	2223	rBV	543826	1143970	45.77%	6.042%
63	8.595	2331	2334	2337	rBV4	1937	1545	0.06%	0.008%
64	8.633	2344	2346	2347	rBV2	1195	450	0.02%	0.002%
65	8.707	2364	2369	2371	rBV4	3317	2532	0.10%	0.013%
66	8.775	2386	2390	2391	rBV4	1070	822	0.03%	0.004%
67	8.785	2391	2393	2394	rVB2	1358	443	0.02%	0.002%
68	8.830	2406	2407	2410	rBV3	904	493	0.02%	0.003%
69	8.891	2414	2426	2452	rBV	1228262	1977215	79.12%	10.443%
70	9.286	2546	2549	2553	rVB4	2297	1690	0.07%	0.009%
71	9.543	2626	2629	2630	rBV3	1110	609	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014093.D
 Acq On : 17 Dec 2019 15:10
 Operator : SY/MD
 Sample : K6276-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.575	2637	2639	2643	rBV4	2118	1671	0.07%	0.009%
73	9.601	2643	2647	2650	rVB5	1914	1373	0.05%	0.007%
74	9.666	2664	2667	2668	rBV3	1031	622	0.02%	0.003%
75	9.704	2677	2679	2681	rVB2	1261	524	0.02%	0.003%
76	9.727	2681	2686	2692	rBV8	1952	1999	0.08%	0.011%
77	9.756	2692	2695	2697	rBV4	1432	1103	0.04%	0.006%
78	9.788	2701	2705	2708	rVB6	1673	1388	0.06%	0.007%
79	9.813	2708	2713	2717	rBV8	1979	2321	0.09%	0.012%
80	9.842	2720	2722	2725	rVV4	924	403	0.02%	0.002%
81	9.887	2734	2736	2740	rBV4	1283	811	0.03%	0.004%
82	9.913	2742	2744	2746	rVB3	1374	452	0.02%	0.002%
83	9.926	2746	2748	2750	rBV2	804	435	0.02%	0.002%
84	9.965	2758	2760	2763	rVV3	1011	532	0.02%	0.003%
85	9.981	2763	2765	2771	rVB6	1255	847	0.03%	0.004%
86	10.006	2771	2773	2777	rVB4	2131	1256	0.05%	0.007%
87	10.035	2777	2782	2784	rBV3	1606	1404	0.06%	0.007%
88	10.074	2792	2794	2799	rVB5	1186	1067	0.04%	0.006%
89	10.109	2799	2805	2808	rBV7	1733	1874	0.07%	0.010%
90	10.125	2808	2810	2814	rVV5	1057	754	0.03%	0.004%
91	10.164	2819	2822	2824	rBV4	756	486	0.02%	0.003%
92	10.254	2838	2850	2870	rBV	765778	1216357	48.67%	6.424%
93	10.772	3009	3011	3014	rBV4	1825	738	0.03%	0.004%
94	11.289	3160	3172	3193	rBV	1091300	1695103	67.83%	8.953%
95	11.665	3278	3289	3306	rBV	1043712	1642338	65.72%	8.674%
96	12.476	3538	3541	3545	rBV6	2025	1633	0.07%	0.009%
97	13.395	3822	3827	3828	rBV4	2379	2000	0.08%	0.011%
98	13.517	3864	3865	3866	rBV	1154	364	0.01%	0.002%
99	14.035	4023	4026	4028	rBV4	1978	1129	0.05%	0.006%
100	14.051	4028	4031	4036	rVV7	1998	1483	0.06%	0.008%


Sum of corrected areas: 18933929

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014093.D
Acq On : 17 Dec 2019 15:10
Operator : SY/MD
Sample : K6276-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

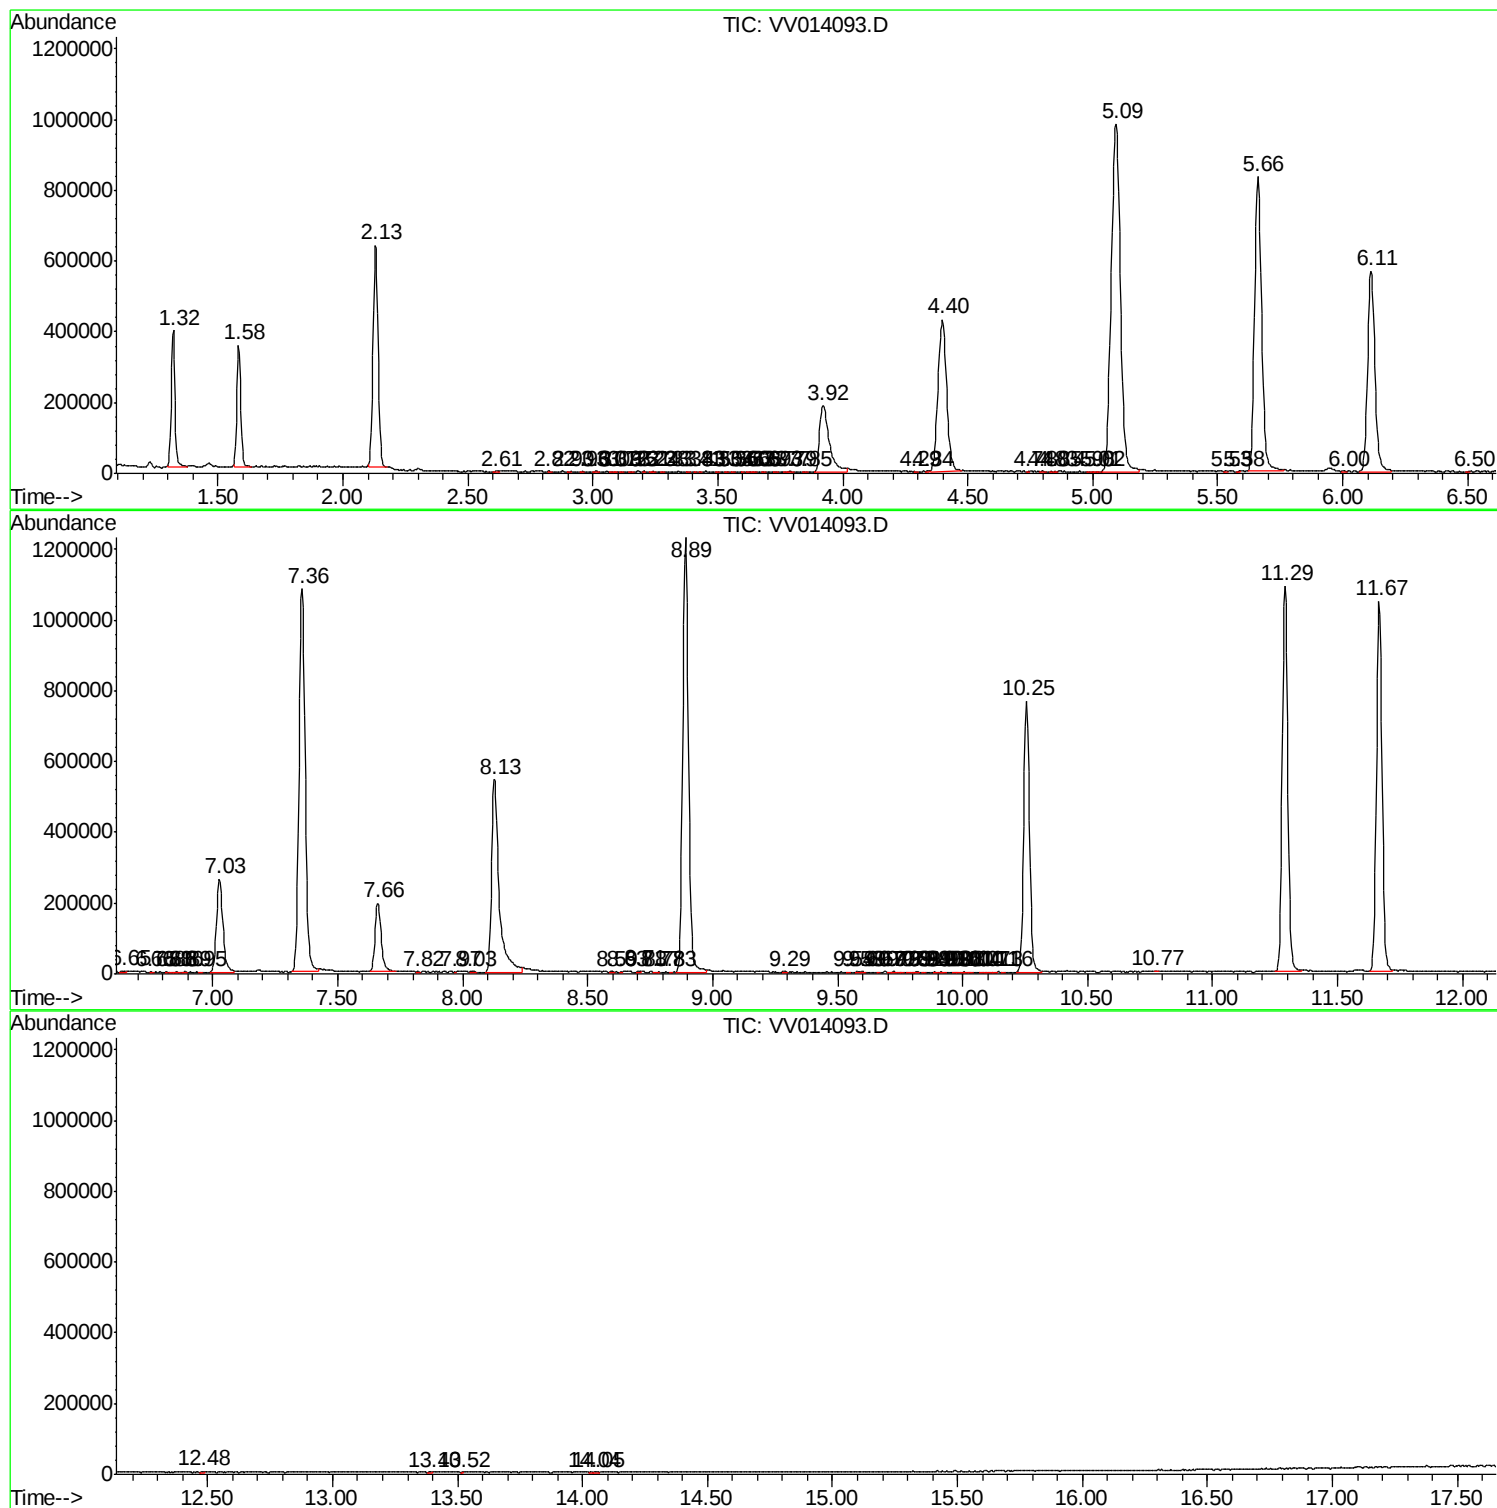

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014093.D
Acq On : 17 Dec 2019 15:10
Operator : SY/MD
Sample : K6276-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C86

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014093.D
Acq On : 17 Dec 2019 15:10
Operator : SY/MD
Sample : K6276-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C86

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc