

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014095.D
 Acq On : 17 Dec 2019 15:57
 Operator : SY/MD
 Sample : K6276-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	82	rVB	387233	373411	15.42%	1.970%
2	1.582	147	153	172	rVB	346308	388024	16.03%	2.047%
3	2.132	315	324	338	rVB	626083	871099	35.98%	4.596%
4	2.753	514	517	519	rBV4	1698	1176	0.05%	0.006%
5	2.849	545	547	551	rBV4	2383	1365	0.06%	0.007%
6	3.145	637	639	640	rBV2	1681	678	0.03%	0.004%
7	3.184	647	651	656	rVB7	1368	1376	0.06%	0.007%
8	3.302	685	688	693	rBV7	3254	1979	0.08%	0.010%
9	3.402	718	719	720	rBV2	1189	444	0.02%	0.002%
10	3.495	744	748	750	rBV4	1906	1389	0.06%	0.007%
11	3.521	754	756	759	rVB4	1929	897	0.04%	0.005%
12	3.547	759	764	765	rBV4	1557	1261	0.05%	0.007%
13	3.856	856	860	864	rBV7	1624	1149	0.05%	0.006%
14	3.872	864	865	866	rBV	911	259	0.01%	0.001%
15	3.923	871	881	913	rVV	174272	460977	19.04%	2.432%
16	4.280	990	992	994	rVB2	1206	391	0.02%	0.002%
17	4.338	1008	1010	1011	rBV2	2036	1024	0.04%	0.005%
18	4.396	1015	1028	1052	rVB	427202	1002907	41.43%	5.291%
19	4.782	1144	1148	1152	rVB7	2191	1756	0.07%	0.009%
20	4.807	1154	1156	1159	rBV4	2305	1672	0.07%	0.009%
21	4.872	1173	1176	1179	rBV4	1322	835	0.03%	0.004%
22	5.093	1225	1245	1267	rBV2	955837	2420904	100.00%	12.773%
23	5.662	1407	1422	1452	rBV	837503	1674495	69.17%	8.835%
24	6.113	1550	1562	1584	rBV	553026	1107718	45.76%	5.844%
25	6.807	1776	1778	1781	rBV4	1946	1302	0.05%	0.007%
26	6.823	1781	1783	1786	rVB3	2138	1180	0.05%	0.006%
27	6.926	1813	1815	1816	rBV2	1473	640	0.03%	0.003%
28	6.968	1826	1828	1834	rVB6	1799	1329	0.05%	0.007%
29	7.026	1834	1846	1865	rBV	270096	490235	20.25%	2.586%
30	7.357	1937	1949	1968	rBV	1097034	1902014	78.57%	10.035%
31	7.659	2034	2043	2063	rBV	198267	338471	13.98%	1.786%
32	7.878	2109	2111	2113	rBV3	1444	845	0.03%	0.004%
33	8.129	2178	2189	2224	rBV	499283	1094108	45.19%	5.773%
34	8.550	2316	2320	2323	rBV5	1647	1325	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014095.D
 Acq On : 17 Dec 2019 15:57
 Operator : SY/MD
 Sample : K6276-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	8.765	2379	2387	2390	rBV5	2560	3336	0.14%	0.018%
36	8.891	2414	2426	2445	rBV	1242344	2008286	82.96%	10.596%
37	9.212	2523	2526	2530	rBV4	1924	1388	0.06%	0.007%
38	9.257	2538	2540	2545	rBV6	1521	1135	0.05%	0.006%
39	9.434	2593	2595	2598	rBV3	1437	1109	0.05%	0.006%
40	9.563	2631	2635	2637	rBV4	1472	1375	0.06%	0.007%
41	9.604	2646	2648	2649	rBV2	1314	485	0.02%	0.003%
42	9.659	2662	2665	2668	rBV4	2150	1360	0.06%	0.007%
43	9.743	2687	2691	2693	rBV4	2216	1845	0.08%	0.010%
44	9.817	2711	2714	2715	rBV3	1307	621	0.03%	0.003%
45	9.871	2727	2731	2733	rBV5	2072	1465	0.06%	0.008%
46	9.968	2759	2761	2762	rBV2	1431	646	0.03%	0.003%
47	10.129	2810	2811	2813	rBV2	1459	407	0.02%	0.002%
48	10.254	2838	2850	2877	rBV	743727	1195847	49.40%	6.309%
49	10.521	2930	2933	2934	rBV3	1248	585	0.02%	0.003%
50	10.530	2934	2936	2937	rBV2	735	212	0.01%	0.001%
51	10.575	2948	2950	2952	rBV3	1600	1001	0.04%	0.005%
52	10.646	2966	2972	2974	rVB6	1809	1405	0.06%	0.007%
53	10.717	2993	2994	2995	rBV	942	234	0.01%	0.001%
54	11.289	3160	3172	3195	rBV	1169451	1820445	75.20%	9.605%
55	11.665	3277	3289	3317	rBV	1110197	1760665	72.73%	9.289%
56	12.604	3579	3581	3586	rVB6	2110	1289	0.05%	0.007%


Sum of corrected areas: 18953776

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014095.D
Acq On : 17 Dec 2019 15:57
Operator : SY/MD
Sample : K6276-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C90

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

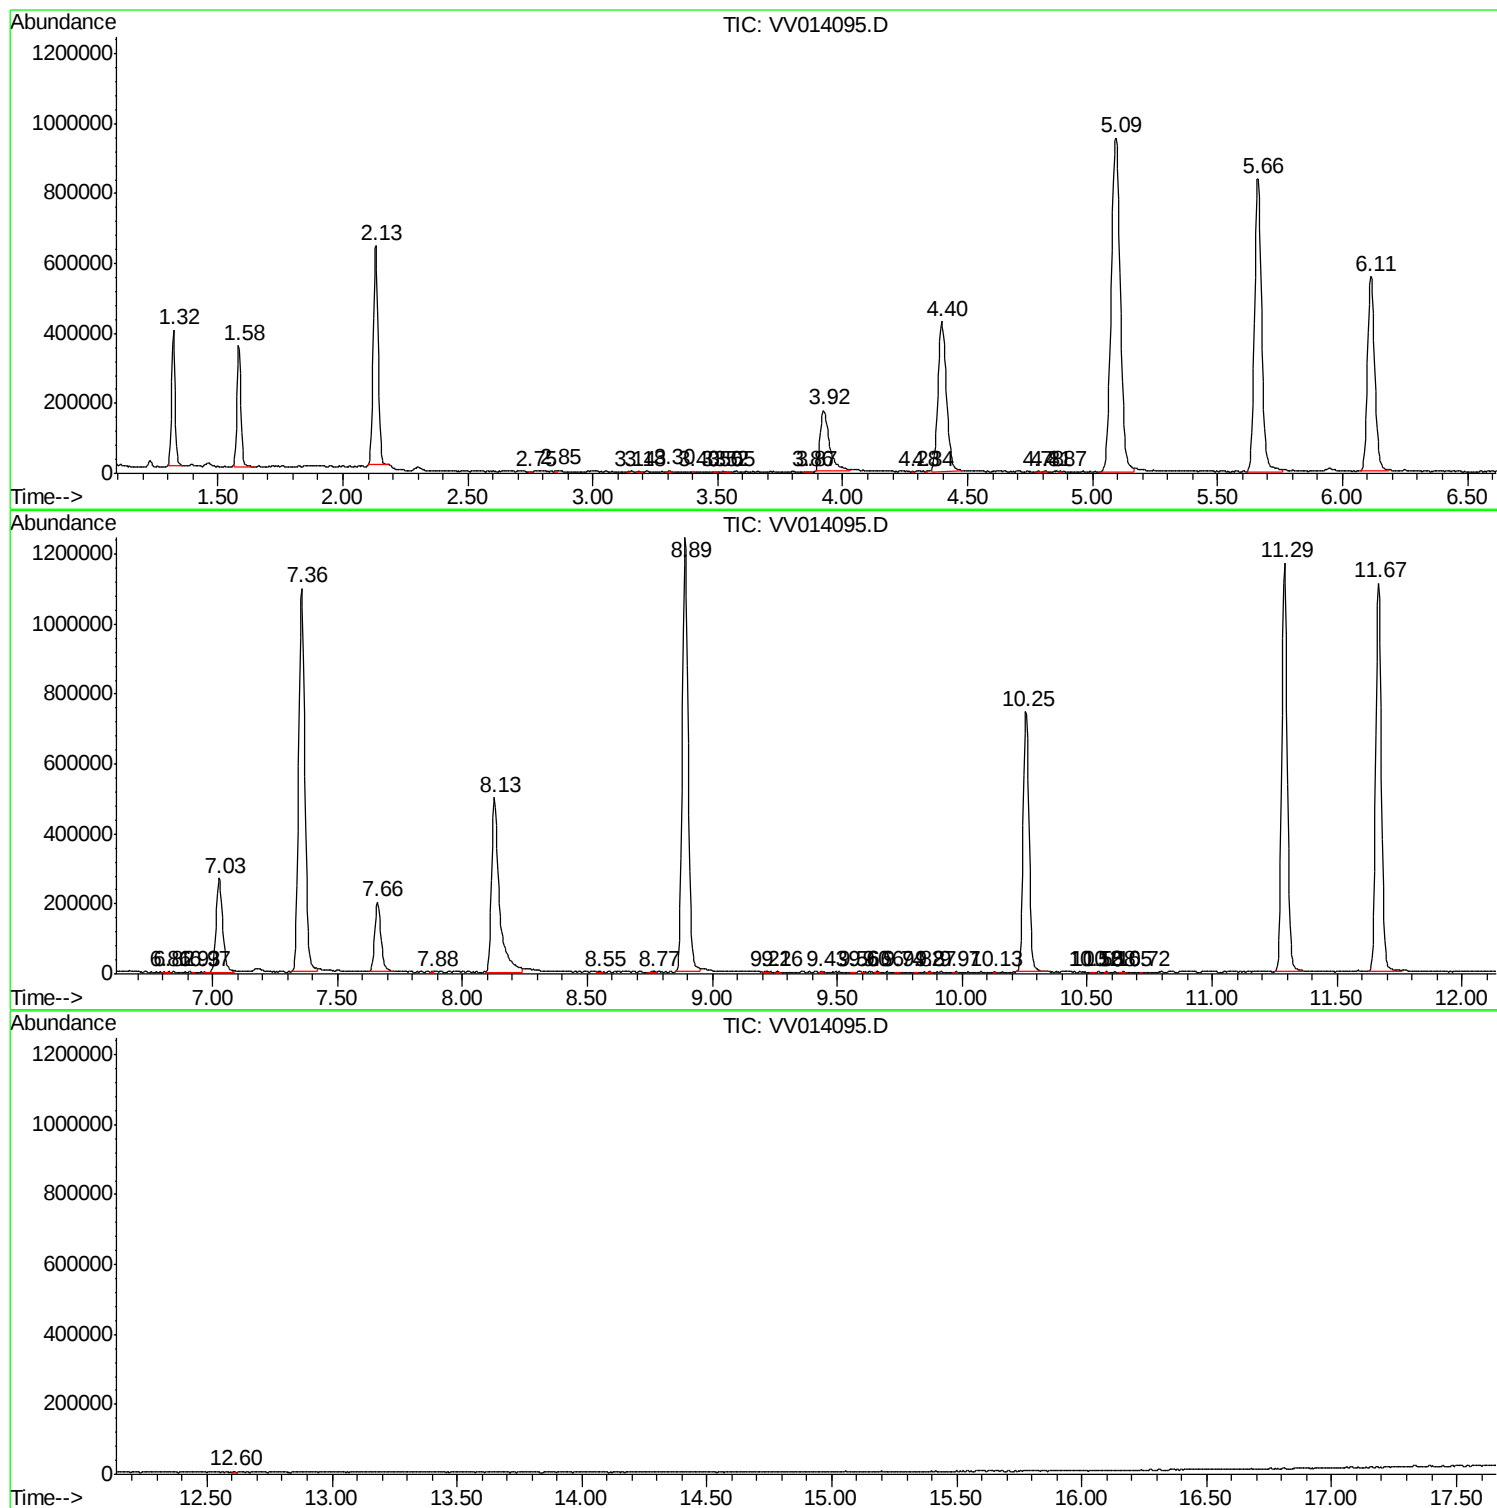

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014095.D
Acq On : 17 Dec 2019 15:57
Operator : SY/MD
Sample : K6276-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C90

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014095.D
Acq On : 17 Dec 2019 15:57
Operator : SY/MD
Sample : K6276-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C90

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc