

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014096.D
 Acq On : 17 Dec 2019 16:21
 Operator : SY/MD
 Sample : K6280-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	40	43	48	rVB	17601	13444	0.55%	0.073%
2	1.322	64	72	84	rBV	379637	378144	15.45%	2.053%
3	1.582	146	153	162	rBV	332751	364082	14.88%	1.977%
4	2.129	314	323	339	rVB	618964	866981	35.43%	4.707%
5	2.270	365	367	369	rBV3	1948	940	0.04%	0.005%
6	2.341	387	389	391	rBV3	1471	999	0.04%	0.005%
7	2.511	439	442	444	rBV3	2324	1441	0.06%	0.008%
8	2.618	471	475	477	rBV4	2004	1424	0.06%	0.008%
9	2.698	497	500	503	rVB5	2050	1026	0.04%	0.006%
10	2.766	517	521	523	rBV3	1745	1107	0.05%	0.006%
11	2.788	526	528	531	rBV3	1743	1020	0.04%	0.006%
12	2.942	571	576	577	rBV4	2026	1120	0.05%	0.006%
13	3.058	609	612	616	rVB5	1818	1099	0.04%	0.006%
14	3.167	644	646	650	rVB5	1300	970	0.04%	0.005%
15	3.283	679	682	684	rBV2	1704	979	0.04%	0.005%
16	3.328	692	696	697	rBV5	1699	1035	0.04%	0.006%
17	3.347	700	702	705	rVB6	2140	1062	0.04%	0.006%
18	3.373	705	710	711	rBV5	2322	2045	0.08%	0.011%
19	3.534	756	760	765	rVB6	1673	1582	0.06%	0.009%
20	3.630	788	790	794	rVB5	1410	942	0.04%	0.005%
21	3.685	803	807	809	rVB4	1697	1072	0.04%	0.006%
22	3.698	809	811	815	rVB5	1615	922	0.04%	0.005%
23	3.749	824	827	830	rBV4	2500	1676	0.07%	0.009%
24	3.827	848	851	854	rVB5	1852	1453	0.06%	0.008%
25	3.923	870	881	910	rBV	177958	471563	19.27%	2.560%
26	4.206	967	969	973	rVB4	2097	1269	0.05%	0.007%
27	4.399	1010	1029	1051	rBV	415652	987153	40.34%	5.360%
28	4.537	1068	1072	1077	rVB7	2383	2363	0.10%	0.013%
29	4.765	1139	1143	1145	rBV3	1317	1067	0.04%	0.006%
30	4.891	1180	1182	1188	rBV6	1683	1658	0.07%	0.009%
31	4.917	1188	1190	1194	rVB4	1634	1028	0.04%	0.006%
32	4.952	1198	1201	1205	rBV4	1241	906	0.04%	0.005%
33	4.974	1205	1208	1210	rBV4	1638	1146	0.05%	0.006%
34	5.093	1224	1245	1274	rBV2	967700	2447369	100.00%	13.288%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014096.D
 Acq On : 17 Dec 2019 16:21
 Operator : SY/MD
 Sample : K6280-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.270	1298	1300	1304	rVB4	1407	979	0.04%	0.005%
36	5.392	1335	1338	1341	rVB3	2856	1898	0.08%	0.010%
37	5.431	1345	1350	1353	rBV7	1840	2229	0.09%	0.012%
38	5.466	1358	1361	1365	rVB5	2688	2017	0.08%	0.011%
39	5.489	1365	1368	1371	rBV5	1527	1329	0.05%	0.007%
40	5.659	1408	1421	1444	rBV	811242	1594240	65.14%	8.656%
41	5.833	1473	1475	1484	rVB8	2552	2478	0.10%	0.013%
42	6.003	1525	1528	1530	rVB4	2219	1143	0.05%	0.006%
43	6.113	1548	1562	1588	rBV	549999	1109186	45.32%	6.022%
44	6.380	1643	1645	1647	rBV3	1622	975	0.04%	0.005%
45	6.447	1660	1666	1668	rBV7	2357	2136	0.09%	0.012%
46	6.482	1672	1677	1679	rBV4	2003	1617	0.07%	0.009%
47	6.492	1679	1680	1685	rVB5	1938	1247	0.05%	0.007%
48	6.524	1687	1690	1694	rBV5	1967	1236	0.05%	0.007%
49	6.653	1721	1730	1734	rBV5	4018	7034	0.29%	0.038%
50	6.859	1792	1794	1797	rVB4	2294	1294	0.05%	0.007%
51	6.884	1797	1802	1803	rBV3	1701	1199	0.05%	0.007%
52	6.913	1808	1811	1812	rVV3	1408	910	0.04%	0.005%
53	6.933	1815	1817	1820	rVB4	1813	968	0.04%	0.005%
54	7.026	1834	1846	1863	rBV	266416	474880	19.40%	2.578%
55	7.148	1881	1884	1886	rBV3	2359	1543	0.06%	0.008%
56	7.222	1905	1907	1910	rVB3	2408	1068	0.04%	0.006%
57	7.357	1934	1949	1965	rBV	1073723	1846829	75.46%	10.027%
58	7.659	2031	2043	2057	rBV	194773	326289	13.33%	1.772%
59	7.836	2094	2098	2102	rVB6	1404	1341	0.05%	0.007%
60	7.859	2102	2105	2108	rBV5	2118	1469	0.06%	0.008%
61	7.923	2121	2125	2129	rVB6	1970	1663	0.07%	0.009%
62	7.965	2135	2138	2140	rBV4	2794	1523	0.06%	0.008%
63	8.055	2162	2166	2167	rBV4	1988	1157	0.05%	0.006%
64	8.129	2178	2189	2227	rBV2	489035	1102134	45.03%	5.984%
65	8.605	2334	2337	2341	rBV5	1588	1320	0.05%	0.007%
66	8.842	2406	2411	2414	rBV7	1788	1739	0.07%	0.009%
67	8.891	2414	2426	2448	rBV	1213540	1933789	79.02%	10.499%
68	9.113	2491	2495	2499	rBV7	1704	1759	0.07%	0.010%
69	9.244	2534	2536	2540	rBV3	1619	1274	0.05%	0.007%
70	9.392	2578	2582	2584	rVB3	2221	1469	0.06%	0.008%
71	9.482	2608	2610	2616	rVB6	2267	1612	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014096.D
 Acq On : 17 Dec 2019 16:21
 Operator : SY/MD
 Sample : K6280-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.537	2624	2627	2629	rBV4	1626	986	0.04%	0.005%
73	9.556	2629	2633	2637	rBV7	1883	1370	0.06%	0.007%
74	9.736	2687	2689	2692	rVB4	1572	981	0.04%	0.005%
75	9.765	2694	2698	2701	rBV4	1859	1571	0.06%	0.009%
76	9.881	2732	2734	2738	rBV4	1884	1234	0.05%	0.007%
77	10.254	2838	2850	2874	rVB	722854	1132834	46.29%	6.151%
78	10.357	2878	2882	2884	rBV4	2931	2209	0.09%	0.012%
79	10.402	2891	2896	2897	rBV5	1826	1611	0.07%	0.009%
80	10.685	2982	2984	2987	rBV4	1323	1041	0.04%	0.006%
81	10.762	3006	3008	3011	rVV3	1629	1057	0.04%	0.006%
82	10.784	3011	3015	3018	rVV5	1252	985	0.04%	0.005%
83	11.022	3086	3089	3090	rBV3	1674	903	0.04%	0.005%
84	11.289	3160	3172	3194	rBV	1050378	1636319	66.86%	8.884%
85	11.537	3246	3249	3251	rBV4	1941	898	0.04%	0.005%
86	11.665	3277	3289	3314	rBV	1014154	1607256	65.67%	8.726%
87	12.501	3547	3549	3554	rBV6	1485	1077	0.04%	0.006%
88	12.595	3575	3578	3583	rVV6	2463	2196	0.09%	0.012%
89	12.620	3584	3586	3591	rVB4	2410	1253	0.05%	0.007%
90	12.797	3638	3641	3642	rBV3	1872	1104	0.05%	0.006%
91	13.447	3841	3843	3849	rVB6	2677	1544	0.06%	0.008%
92	13.524	3861	3867	3870	rBV8	2527	2833	0.12%	0.015%
93	13.649	3903	3906	3911	rVB7	1702	1036	0.04%	0.006%
94	13.852	3967	3969	3973	rBV4	2361	1308	0.05%	0.007%
95	13.958	4000	4002	4004	rBV3	1672	1070	0.04%	0.006%
96	14.640	4211	4214	4217	rBV4	1863	1135	0.05%	0.006%
97	14.749	4246	4248	4251	rVB3	2096	1277	0.05%	0.007%
98	14.810	4265	4267	4270	rBV4	2054	1486	0.06%	0.008%
99	14.845	4276	4278	4280	rBV3	2022	1033	0.04%	0.006%
100	17.157	4994	4997	5001	rVB	16998	9809	0.40%	0.053%


Sum of corrected areas: 18418476

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014096.D
Acq On : 17 Dec 2019 16:21
Operator : SY/MD
Sample : K6280-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF30

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

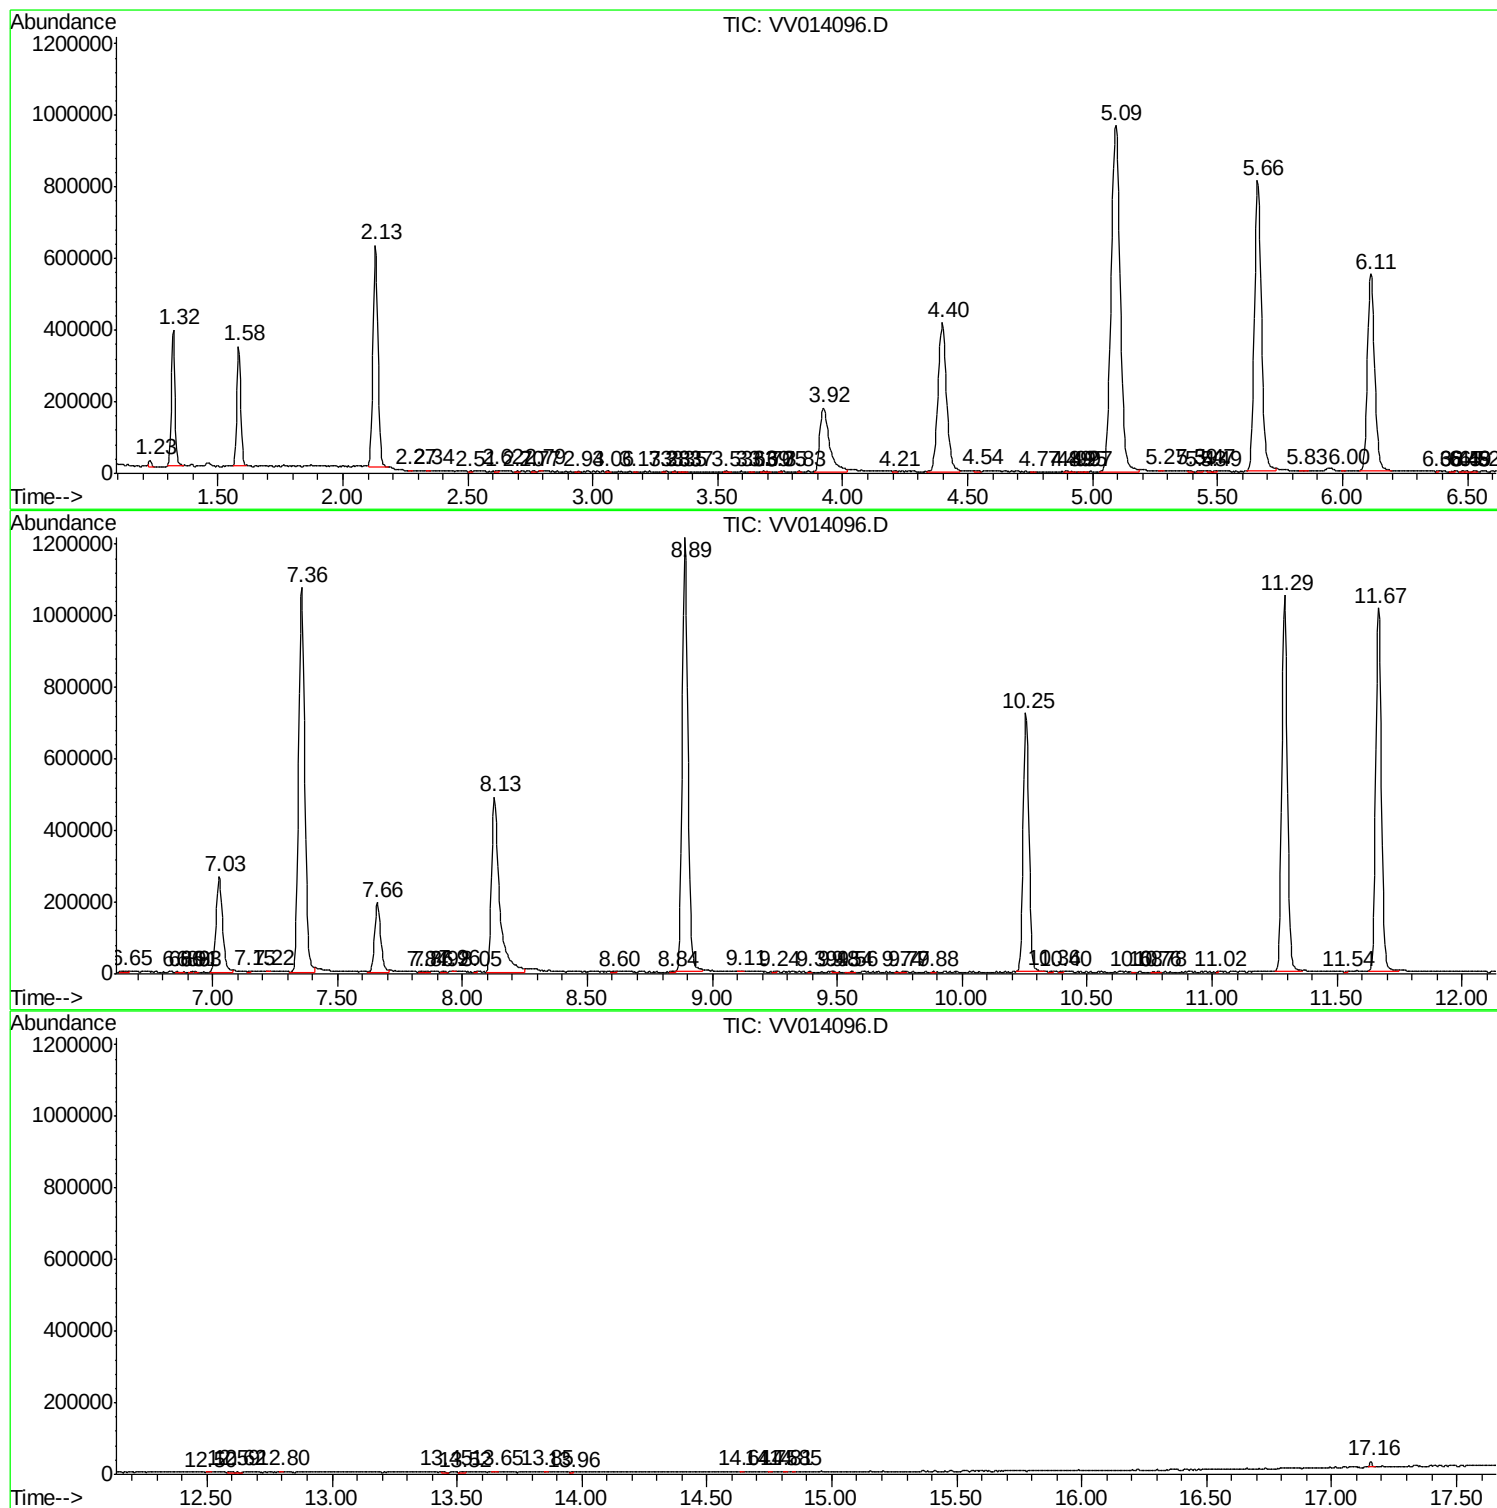

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014096.D
Acq On : 17 Dec 2019 16:21
Operator : SY/MD
Sample : K6280-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF30

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014096.D
Acq On : 17 Dec 2019 16:21
Operator : SY/MD
Sample : K6280-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF30

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc