

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014099.D
 Acq On : 17 Dec 2019 17:32
 Operator : SY/MD
 Sample : K6280-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	83	rBV	396250	385178	15.43%	2.027%
2	1.582	147	153	169	rVB	344036	384929	15.42%	2.025%
3	2.132	315	324	337	rVB	620862	862267	34.54%	4.537%
4	2.508	439	441	443	rBV3	1418	905	0.04%	0.005%
5	2.672	491	492	495	rBV3	1002	464	0.02%	0.002%
6	2.695	495	499	500	rBV4	1441	751	0.03%	0.004%
7	2.736	505	512	515	rBV7	2134	2591	0.10%	0.014%
8	2.772	521	523	525	rBV3	1438	918	0.04%	0.005%
9	2.859	547	550	551	rBV3	1457	914	0.04%	0.005%
10	2.926	569	571	574	rBV2	1591	1017	0.04%	0.005%
11	2.965	582	583	586	rVB3	1510	485	0.02%	0.003%
12	2.984	586	589	591	rVB3	1163	648	0.03%	0.003%
13	3.003	591	595	597	rBV4	2364	1907	0.08%	0.010%
14	3.074	614	617	619	rBV5	1036	604	0.02%	0.003%
15	3.154	638	642	644	rVB4	1937	1345	0.05%	0.007%
16	3.171	644	647	648	rBV3	1128	628	0.03%	0.003%
17	3.196	653	655	657	rBV3	1899	972	0.04%	0.005%
18	3.235	665	667	668	rVB2	1155	398	0.02%	0.002%
19	3.257	668	674	675	rBV4	1414	1130	0.05%	0.006%
20	3.322	692	694	696	rBV3	1408	465	0.02%	0.002%
21	3.344	696	701	705	rBV7	1683	2009	0.08%	0.011%
22	3.470	738	740	742	rBV2	1144	629	0.03%	0.003%
23	3.495	744	748	752	rVB7	1427	1349	0.05%	0.007%
24	3.515	752	754	757	rBV4	848	420	0.02%	0.002%
25	3.550	761	765	766	rBV3	1349	870	0.03%	0.005%
26	3.563	766	769	772	rVB5	1567	915	0.04%	0.005%
27	3.707	812	814	816	rBV3	888	495	0.02%	0.003%
28	3.743	823	825	826	rBV2	1388	635	0.03%	0.003%
29	3.781	834	837	840	rBV4	1131	1079	0.04%	0.006%
30	3.923	869	881	914	rBV	185733	503615	20.17%	2.650%
31	4.399	1014	1029	1055	rVB	423131	1000215	40.06%	5.263%
32	4.624	1096	1099	1102	rBV4	1663	1449	0.06%	0.008%
33	4.769	1142	1144	1146	rBV3	1230	617	0.02%	0.003%
34	4.807	1154	1156	1158	rBV2	1128	717	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014099.D
 Acq On : 17 Dec 2019 17:32
 Operator : SY/MD
 Sample : K6280-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.865	1172	1174	1177	rVB3	1277	569	0.02%	0.003%
36	4.884	1177	1180	1183	rVB4	1107	846	0.03%	0.004%
37	4.907	1184	1187	1189	rBV3	1114	649	0.03%	0.003%
38	5.006	1215	1218	1219	rBV3	1177	727	0.03%	0.004%
39	5.019	1219	1222	1223	rVV3	1435	690	0.03%	0.004%
40	5.093	1227	1245	1269	rBV2	986957	2496549	100.00%	13.136%
41	5.405	1340	1342	1344	rBV3	1365	574	0.02%	0.003%
42	5.556	1387	1389	1390	rBV2	1285	659	0.03%	0.003%
43	5.662	1408	1422	1451	rBV	810071	1634766	65.48%	8.602%
44	6.006	1528	1529	1533	rVB4	1896	777	0.03%	0.004%
45	6.116	1549	1563	1584	rBV	558669	1133306	45.39%	5.963%
46	6.347	1631	1635	1640	rVB6	2125	2209	0.09%	0.012%
47	6.444	1662	1665	1668	rBV4	1896	1484	0.06%	0.008%
48	6.547	1692	1697	1698	rBV4	1561	979	0.04%	0.005%
49	6.579	1706	1707	1711	rVB3	1688	735	0.03%	0.004%
50	6.601	1711	1714	1715	rBV3	934	498	0.02%	0.003%
51	6.897	1803	1806	1808	rBV4	1046	491	0.02%	0.003%
52	6.955	1821	1824	1825	rBV3	1046	458	0.02%	0.002%
53	7.026	1834	1846	1869	rVV	264128	485510	19.45%	2.555%
54	7.357	1936	1949	1968	rBV	1110461	1921427	76.96%	10.110%
55	7.595	2021	2023	2025	rBV3	2437	1165	0.05%	0.006%
56	7.659	2033	2043	2059	rBV2	194156	329877	13.21%	1.736%
57	7.923	2123	2125	2127	rBV3	1493	625	0.03%	0.003%
58	8.042	2157	2162	2166	rBV7	2147	2265	0.09%	0.012%
59	8.129	2178	2189	2222	rBV	520196	1131572	45.33%	5.954%
60	8.460	2288	2292	2293	rBV4	2628	2013	0.08%	0.011%
61	8.501	2303	2305	2310	rBV6	1890	1371	0.05%	0.007%
62	8.842	2409	2411	2414	rBV5	1599	831	0.03%	0.004%
63	8.891	2414	2426	2443	rBV	1203379	1970958	78.95%	10.371%
64	9.100	2488	2491	2494	rBV4	1963	1385	0.06%	0.007%
65	9.302	2550	2554	2557	rBV5	995	938	0.04%	0.005%
66	9.357	2568	2571	2574	rVB3	1506	815	0.03%	0.004%
67	9.395	2580	2583	2584	rBV2	1749	659	0.03%	0.003%
68	9.508	2616	2618	2621	rVB3	1861	1005	0.04%	0.005%
69	9.530	2621	2625	2627	rBV4	2344	1526	0.06%	0.008%
70	9.640	2656	2659	2664	rBV6	2206	1579	0.06%	0.008%
71	9.698	2674	2677	2679	rVB3	1198	613	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014099.D
 Acq On : 17 Dec 2019 17:32
 Operator : SY/MD
 Sample : K6280-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.727	2682	2686	2689	rBV5	1345	1163	0.05%	0.006%
73	9.807	2709	2711	2714	rVB4	1832	673	0.03%	0.004%
74	9.845	2719	2723	2725	rBV4	1316	1067	0.04%	0.006%
75	9.910	2738	2743	2748	rBV8	1945	2446	0.10%	0.013%
76	9.981	2763	2765	2769	rBV3	2048	1380	0.06%	0.007%
77	10.035	2780	2782	2784	rBV3	1584	766	0.03%	0.004%
78	10.048	2784	2786	2788	rVB3	1956	863	0.03%	0.005%
79	10.064	2788	2791	2793	rBV3	1430	894	0.04%	0.005%
80	10.116	2804	2807	2811	rBV5	1940	1625	0.07%	0.009%
81	10.151	2815	2818	2820	rBV3	1215	899	0.04%	0.005%
82	10.254	2838	2850	2870	rBV	754920	1207832	48.38%	6.355%
83	10.498	2923	2926	2927	rBV3	1107	771	0.03%	0.004%
84	10.553	2940	2943	2944	rBV3	1476	660	0.03%	0.003%
85	10.961	3067	3070	3072	rBV4	1767	1131	0.05%	0.006%
86	11.122	3116	3120	3123	rBV6	1430	1267	0.05%	0.007%
87	11.164	3131	3133	3135	rBV3	1643	902	0.04%	0.005%
88	11.289	3160	3172	3190	rBV	1114075	1736466	69.55%	9.137%
89	11.665	3277	3289	3312	rBV	1107035	1733416	69.43%	9.121%
90	12.144	3436	3438	3439	rBV	1954	832	0.03%	0.004%
91	12.890	3666	3670	3673	rBV5	2090	1936	0.08%	0.010%
92	13.067	3722	3725	3727	rBV4	2425	1966	0.08%	0.010%
93	13.302	3796	3798	3800	rBV3	1828	712	0.03%	0.004%
94	13.431	3836	3838	3840	rBV3	2082	1142	0.05%	0.006%
95	13.617	3894	3896	3899	rBV3	1993	1150	0.05%	0.006%
96	13.704	3919	3923	3925	rBV4	2046	1712	0.07%	0.009%
97	13.897	3981	3983	3985	rBV3	1689	807	0.03%	0.004%
98	13.939	3992	3996	4001	rBV5	2379	2361	0.09%	0.012%
99	13.996	4012	4014	4015	rBV2	1262	425	0.02%	0.002%
100	14.585	4195	4197	4199	rBV3	1970	999	0.04%	0.005%


Sum of corrected areas: 19004893

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014099.D
Acq On : 17 Dec 2019 17:32
Operator : SY/MD
Sample : K6280-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF33

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

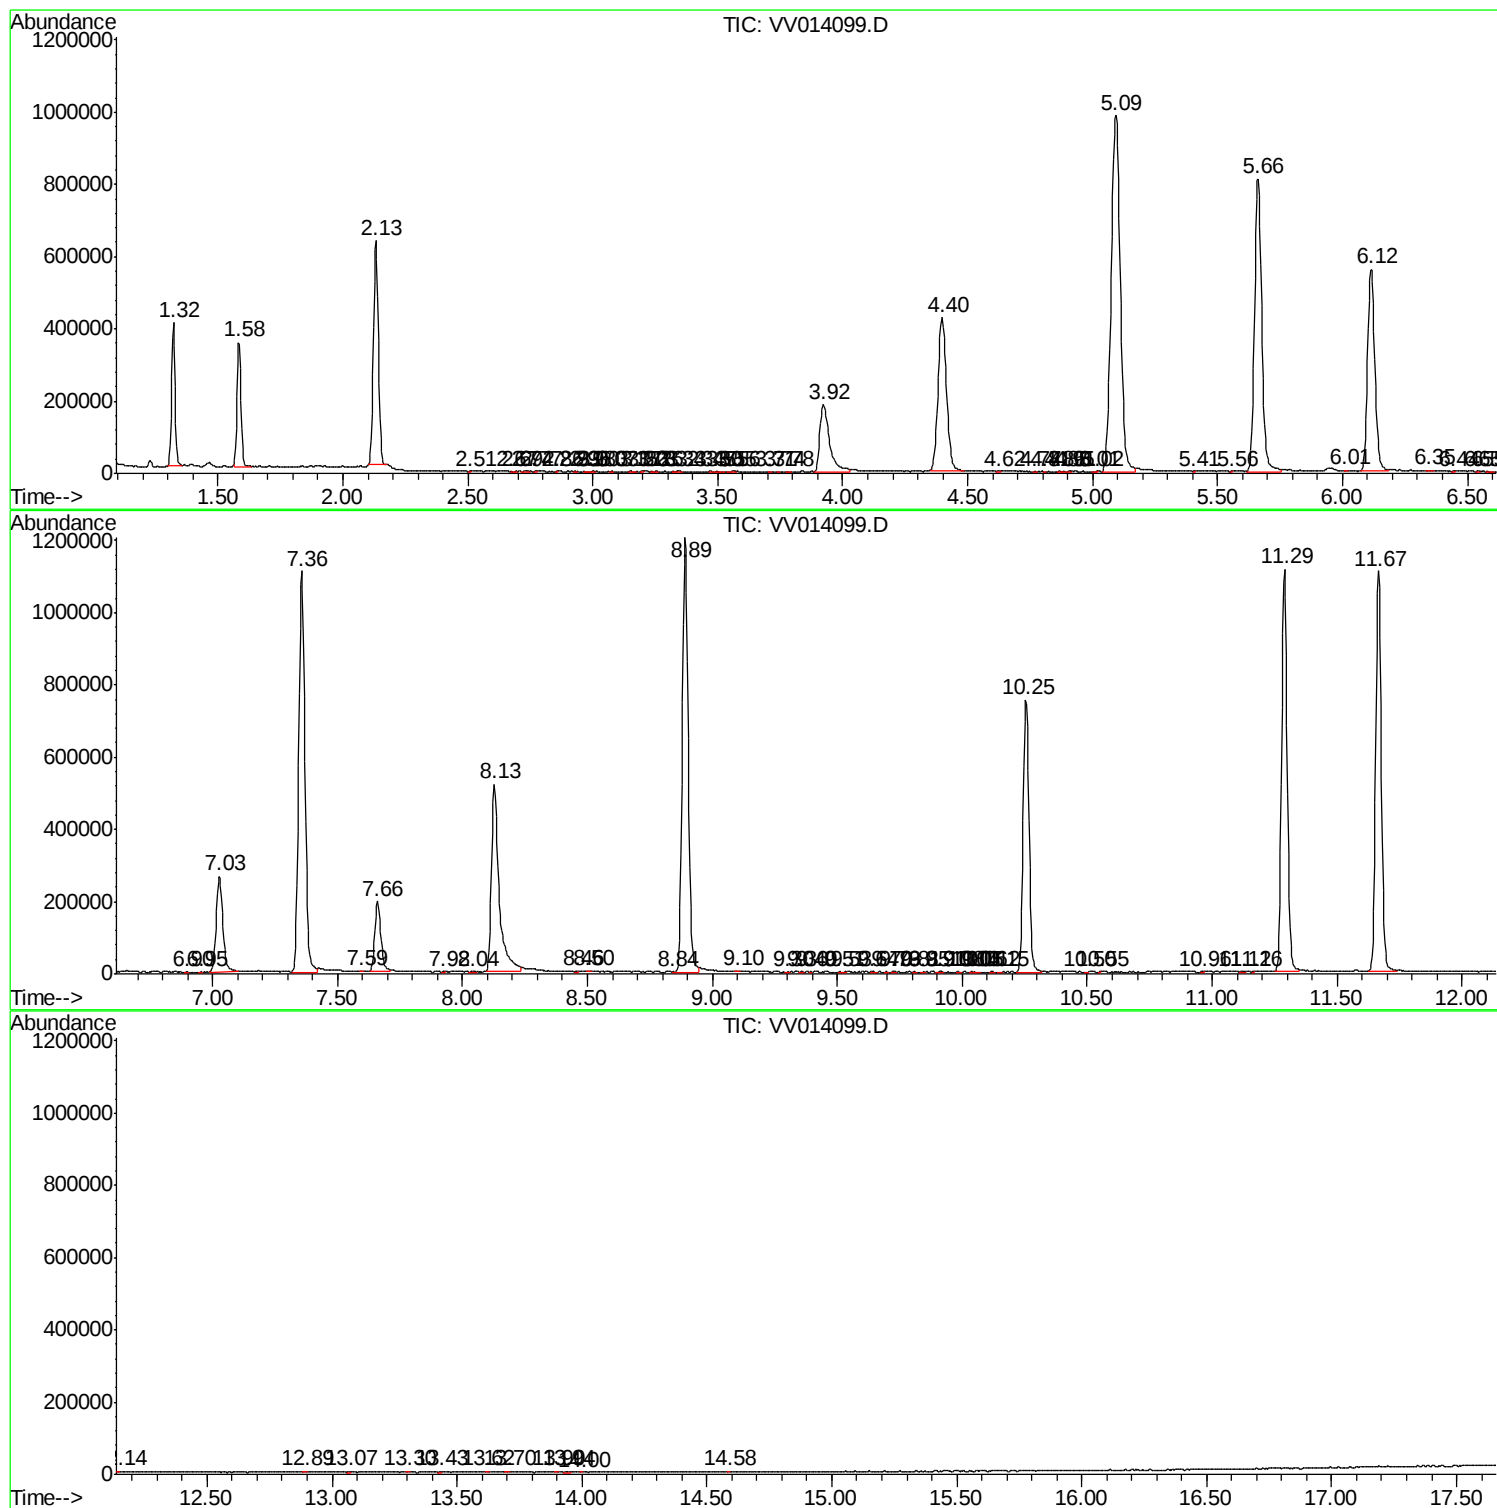

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014099.D
Acq On : 17 Dec 2019 17:32
Operator : SY/MD
Sample : K6280-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF33

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014099.D
Acq On : 17 Dec 2019 17:32
Operator : SY/MD
Sample : K6280-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF33

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc