

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014100.D
 Acq On : 17 Dec 2019 17:56
 Operator : SY/MD
 Sample : K6280-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	84	rVB	379552	375586	15.29%	1.996%
2	1.582	147	153	165	rVB	343682	383149	15.60%	2.036%
3	2.132	315	324	351	rVB	621724	935062	38.07%	4.970%
4	2.573	459	461	463	rBV3	1966	876	0.04%	0.005%
5	2.627	474	478	480	rBV4	2191	1414	0.06%	0.008%
6	2.913	564	567	569	rBV3	1547	875	0.04%	0.005%
7	2.946	575	577	579	rBV3	1281	795	0.03%	0.004%
8	3.016	597	599	600	rBV2	1154	459	0.02%	0.002%
9	3.058	610	612	616	rVB5	1977	1119	0.05%	0.006%
10	3.084	618	620	624	rVB4	2014	1251	0.05%	0.007%
11	3.135	633	636	641	rBV7	2124	1559	0.06%	0.008%
12	3.193	652	654	655	rBV2	542	158	0.01%	0.001%
13	3.203	655	657	659	rVB3	1277	409	0.02%	0.002%
14	3.219	659	662	664	rBV4	2195	1345	0.05%	0.007%
15	3.235	665	667	669	rBV3	1067	514	0.02%	0.003%
16	3.296	684	686	688	rBV3	1318	630	0.03%	0.003%
17	3.328	693	696	699	rVB4	2076	1478	0.06%	0.008%
18	3.347	699	702	704	rBV2	1675	930	0.04%	0.005%
19	3.360	704	706	710	rBV4	2566	1392	0.06%	0.007%
20	3.405	717	720	722	rBV4	1397	642	0.03%	0.003%
21	3.434	726	729	731	rBV4	966	589	0.02%	0.003%
22	3.508	750	752	754	rVB3	2746	1022	0.04%	0.005%
23	3.524	754	757	759	rBV3	1242	930	0.04%	0.005%
24	3.560	764	768	770	rVB5	1214	822	0.03%	0.004%
25	3.820	848	849	850	rBV2	1081	274	0.01%	0.001%
26	3.923	870	881	905	rBV	170264	453200	18.45%	2.409%
27	4.396	1010	1028	1055	rBV2	419941	1017989	41.44%	5.411%
28	4.714	1123	1127	1131	rBV6	1531	1772	0.07%	0.009%
29	4.772	1143	1145	1148	rBV3	1617	952	0.04%	0.005%
30	4.872	1174	1176	1181	rBV3	1661	1113	0.05%	0.006%
31	4.894	1181	1183	1184	rBV2	1164	473	0.02%	0.003%
32	4.978	1206	1209	1210	rBV2	1340	710	0.03%	0.004%
33	5.013	1217	1220	1224	rBV4	2348	2181	0.09%	0.012%
34	5.032	1224	1226	1227	rVV2	1375	586	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014100.D
 Acq On : 17 Dec 2019 17:56
 Operator : SY/MD
 Sample : K6280-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.093	1227	1245	1271	rVV2	979729	2456256	100.00%	13.055%
36	5.553	1386	1388	1392	rVB4	1842	993	0.04%	0.005%
37	5.659	1407	1421	1447	rBV	797518	1592630	64.84%	8.465%
38	5.900	1495	1496	1498	rBV2	1516	666	0.03%	0.004%
39	6.113	1550	1562	1583	rBV	543531	1087476	44.27%	5.780%
40	6.505	1682	1684	1688	rBV5	2620	1927	0.08%	0.010%
41	6.791	1771	1773	1775	rVB2	1146	330	0.01%	0.002%
42	6.807	1775	1778	1781	rBV4	1391	846	0.03%	0.004%
43	6.865	1794	1796	1800	rBV4	2446	1719	0.07%	0.009%
44	7.026	1835	1846	1864	rBV	260300	471497	19.20%	2.506%
45	7.357	1936	1949	1969	rBV	1105772	1899700	77.34%	10.097%
46	7.659	2034	2043	2061	rBV	194658	322309	13.12%	1.713%
47	7.981	2133	2143	2150	rBV	5120	10764	0.44%	0.057%
48	8.129	2179	2189	2215	rBV	498072	1045841	42.58%	5.559%
49	8.781	2389	2392	2394	rVB4	1462	860	0.04%	0.005%
50	8.842	2409	2411	2413	rBV3	1807	869	0.04%	0.005%
51	8.891	2414	2426	2447	rVV	1236152	1989523	81.00%	10.574%
52	9.383	2577	2579	2584	rBV5	1480	973	0.04%	0.005%
53	9.402	2584	2585	2587	rBV2	1123	438	0.02%	0.002%
54	9.466	2602	2605	2607	rBV3	1719	1001	0.04%	0.005%
55	9.498	2613	2615	2616	rBV2	1272	379	0.02%	0.002%
56	9.582	2637	2641	2643	rBV3	1347	946	0.04%	0.005%
57	9.662	2665	2666	2668	rVB2	1309	312	0.01%	0.002%
58	9.678	2669	2671	2674	rVB3	2498	1346	0.05%	0.007%
59	9.694	2674	2676	2678	rBV3	1607	905	0.04%	0.005%
60	9.743	2688	2691	2692	rBV3	860	541	0.02%	0.003%
61	9.756	2692	2695	2696	rBV3	1279	793	0.03%	0.004%
62	9.842	2718	2722	2724	rBV5	1492	1181	0.05%	0.006%
63	9.884	2733	2735	2737	rBV3	1163	582	0.02%	0.003%
64	9.948	2752	2755	2758	rVB5	1185	557	0.02%	0.003%
65	10.019	2775	2777	2778	rVB2	1483	423	0.02%	0.002%
66	10.093	2796	2800	2802	rBV5	1994	1443	0.06%	0.008%
67	10.157	2817	2820	2822	rBV4	2226	1179	0.05%	0.006%
68	10.202	2832	2834	2837	rBV4	1042	686	0.03%	0.004%
69	10.254	2840	2850	2872	rVB	750641	1182117	48.13%	6.283%
70	10.514	2927	2931	2933	rBV5	1758	1099	0.04%	0.006%
71	10.530	2933	2936	2939	rVV4	2095	1627	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014100.D
 Acq On : 17 Dec 2019 17:56
 Operator : SY/MD
 Sample : K6280-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.595	2950	2956	2959	rBV5	2254	2164	0.09%	0.012%
73	10.611	2959	2961	2963	rVB3	1423	482	0.02%	0.003%
74	10.669	2976	2979	2982	rVB3	1634	973	0.04%	0.005%
75	10.688	2982	2985	2986	rBV3	1257	727	0.03%	0.004%
76	10.749	3001	3004	3007	rBV4	1122	1019	0.04%	0.005%
77	10.797	3015	3019	3021	rBV3	1871	1470	0.06%	0.008%
78	10.858	3036	3038	3041	rBV3	1197	808	0.03%	0.004%
79	10.997	3079	3081	3082	rBV2	1427	537	0.02%	0.003%
80	11.071	3103	3104	3108	rBV3	1051	814	0.03%	0.004%
81	11.129	3119	3122	3124	rBV2	1760	1078	0.04%	0.006%
82	11.202	3143	3145	3146	rBV3	1922	823	0.03%	0.004%
83	11.289	3160	3172	3193	rBV	1167390	1803819	73.44%	9.587%
84	11.665	3277	3289	3305	rBV	1090295	1719646	70.01%	9.140%
85	11.990	3387	3390	3391	rBV3	1978	1232	0.05%	0.007%
86	13.302	3795	3798	3800	rBV3	2107	1398	0.06%	0.007%
87	13.675	3912	3914	3917	rBV3	2183	1525	0.06%	0.008%
88	13.948	3997	3999	4000	rBV2	1975	982	0.04%	0.005%


Sum of corrected areas: 18814487

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014100.D
Acq On : 17 Dec 2019 17:56
Operator : SY/MD
Sample : K6280-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

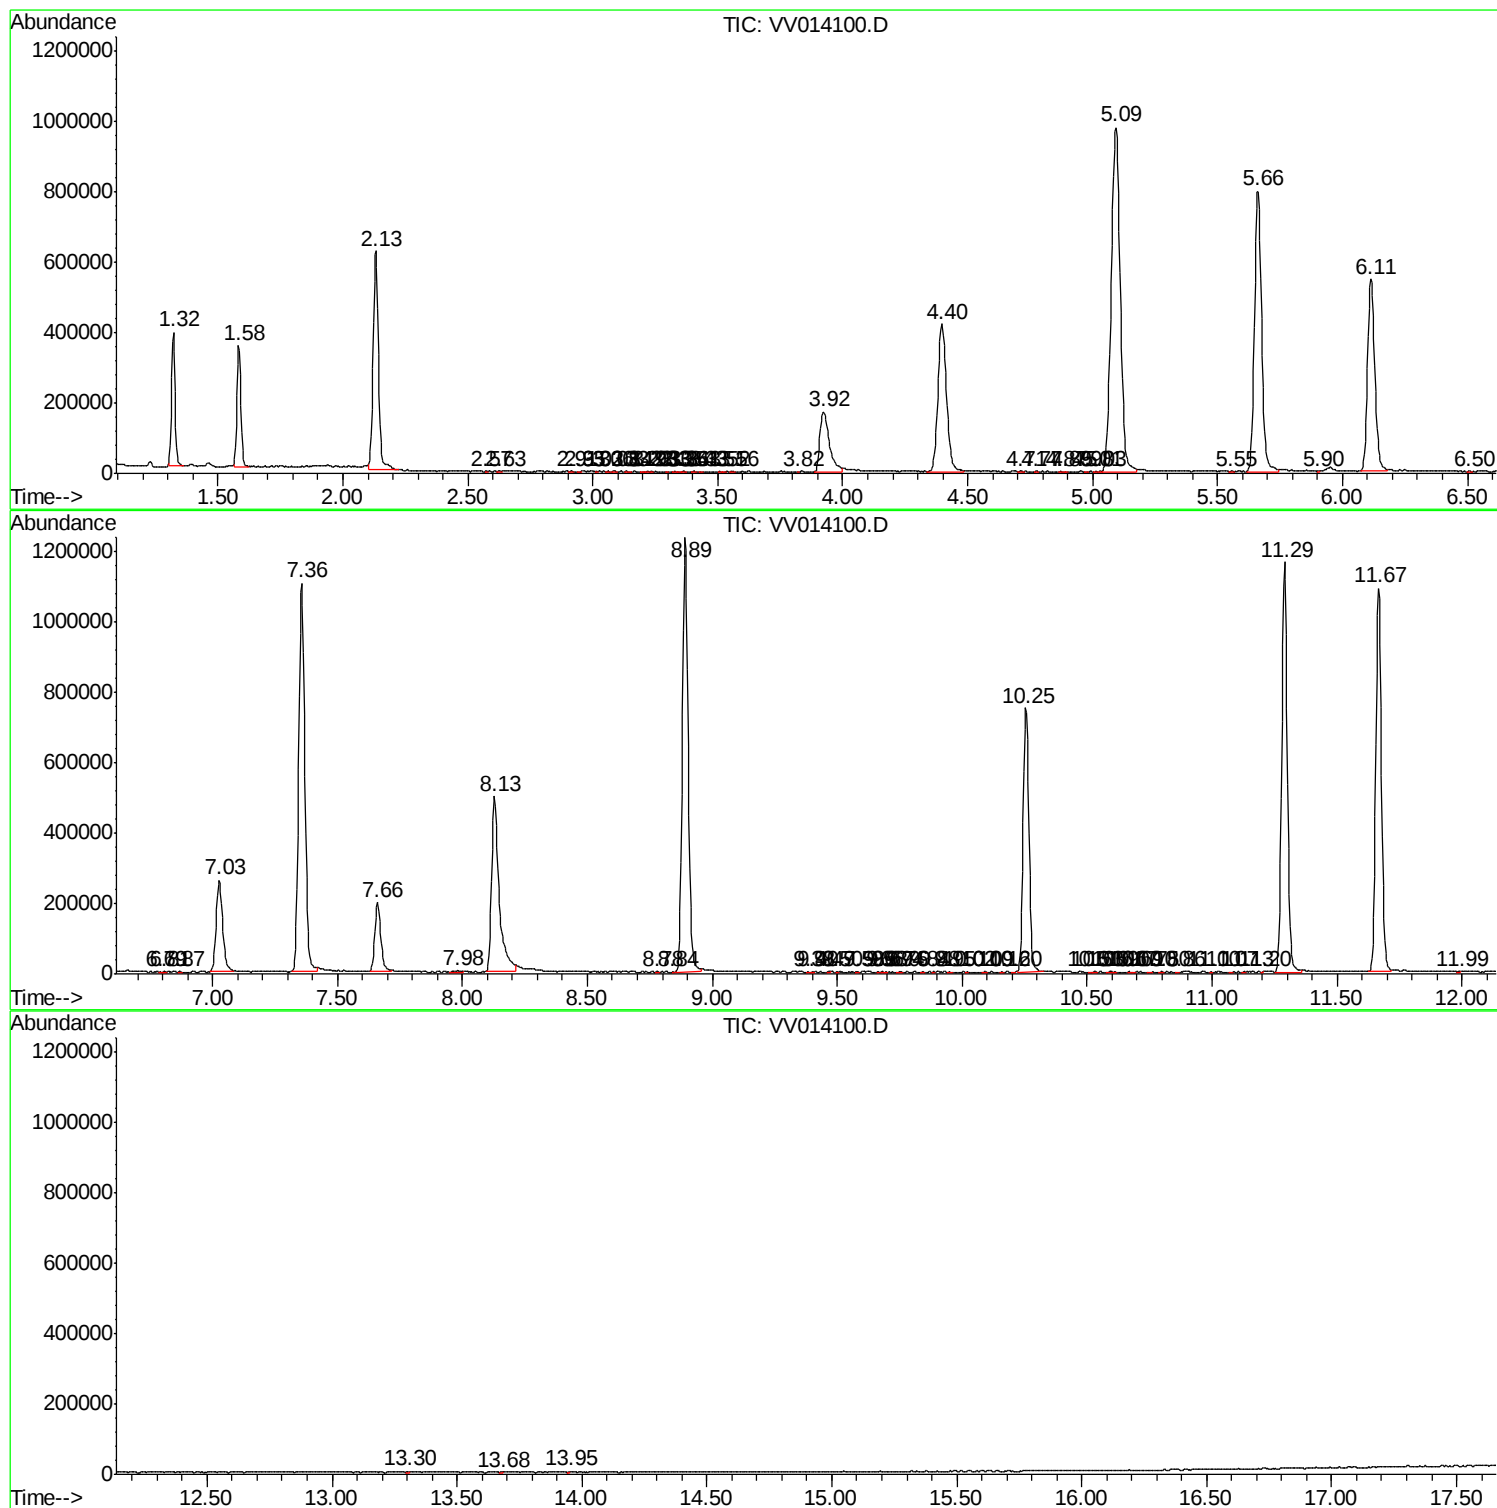

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014100.D
Acq On : 17 Dec 2019 17:56
Operator : SY/MD
Sample : K6280-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF36

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014100.D
Acq On : 17 Dec 2019 17:56
Operator : SY/MD
Sample : K6280-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF36

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc