

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014102.D
 Acq On : 17 Dec 2019 18:43
 Operator : SY/MD
 Sample : K6314-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.145	12	17	24	rVB	46159	45313	1.82%	0.235%
2	1.322	65	72	86	rVB	391352	387128	15.56%	2.005%
3	1.582	146	153	164	rVB	343414	379779	15.26%	1.967%
4	2.132	314	324	352	rVB	634771	939396	37.75%	4.866%
5	2.460	421	426	429	rVB8	2201	2045	0.08%	0.011%
6	2.483	429	433	435	rBV4	1478	1068	0.04%	0.006%
7	2.605	468	471	474	rBV4	1539	1305	0.05%	0.007%
8	2.920	564	569	575	rVB10	1760	2028	0.08%	0.011%
9	3.116	626	630	638	rBV10	2061	3066	0.12%	0.016%
10	3.151	638	641	643	rBV4	1878	1323	0.05%	0.007%
11	3.283	677	682	685	rBV6	1859	1465	0.06%	0.008%
12	3.393	711	716	718	rBV5	1726	1196	0.05%	0.006%
13	3.708	810	814	820	rBV9	2313	2938	0.12%	0.015%
14	3.769	830	833	837	rVB7	1779	1106	0.04%	0.006%
15	3.794	837	841	846	rBV8	2706	2965	0.12%	0.015%
16	3.923	870	881	907	rBV	179496	473444	19.03%	2.452%
17	4.093	931	934	937	rBV4	1835	1122	0.05%	0.006%
18	4.399	1012	1029	1051	rBV	416591	1024718	41.18%	5.308%
19	4.544	1071	1074	1076	rBV4	1860	1386	0.06%	0.007%
20	4.656	1107	1109	1114	rVB5	1730	1338	0.05%	0.007%
21	4.807	1153	1156	1161	rVB5	3253	2654	0.11%	0.014%
22	4.849	1161	1169	1175	rBV5	2387	3766	0.15%	0.020%
23	5.093	1225	1245	1269	rBV2	980960	2488160	100.00%	12.888%
24	5.434	1347	1351	1353	rBV5	2118	1524	0.06%	0.008%
25	5.663	1407	1422	1454	rVV	817776	1633527	65.65%	8.461%
26	5.946	1499	1510	1519	rBV	9440	20899	0.84%	0.108%
27	6.016	1530	1532	1535	rVB4	2286	1361	0.05%	0.007%
28	6.113	1546	1562	1582	rBV	546582	1116782	44.88%	5.784%
29	6.360	1637	1639	1644	rVV5	2025	1341	0.05%	0.007%
30	6.383	1644	1646	1651	rVB4	2496	2092	0.08%	0.011%
31	6.560	1696	1701	1706	rVV9	2272	2635	0.11%	0.014%
32	6.650	1720	1729	1732	rBV10	4637	6856	0.28%	0.036%
33	6.807	1775	1778	1781	rBV5	1984	1286	0.05%	0.007%
34	6.865	1794	1796	1802	rVB7	1899	1191	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014102.D
 Acq On : 17 Dec 2019 18:43
 Operator : SY/MD
 Sample : K6314-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.942	1818	1820	1823	rBV4	2016	1267	0.05%	0.007%
36	6.962	1823	1826	1829	rBV3	2054	1743	0.07%	0.009%
37	7.026	1834	1846	1864	rBV	267336	472843	19.00%	2.449%
38	7.238	1909	1912	1918	rVB8	2194	2172	0.09%	0.011%
39	7.357	1937	1949	1968	rBV	1105120	1894157	76.13%	9.811%
40	7.659	2032	2043	2059	rBV	196257	338882	13.62%	1.755%
41	8.129	2177	2189	2223	rBV	518984	1127252	45.30%	5.839%
42	8.460	2290	2292	2295	rBV3	1645	1240	0.05%	0.006%
43	8.553	2318	2321	2324	rVB5	1934	1274	0.05%	0.007%
44	8.717	2369	2372	2379	rVB9	3396	4079	0.16%	0.021%
45	8.752	2379	2383	2384	rBV3	1567	1153	0.05%	0.006%
46	8.891	2411	2426	2456	rBV	1257541	2036263	81.84%	10.547%
47	9.048	2473	2475	2481	rBV6	1863	1716	0.07%	0.009%
48	9.228	2526	2531	2533	rBV5	1773	1578	0.06%	0.008%
49	9.402	2581	2585	2587	rBV4	1583	1360	0.05%	0.007%
50	9.473	2603	2607	2609	rBV5	1636	1455	0.06%	0.008%
51	9.547	2625	2630	2631	rBV4	2440	1751	0.07%	0.009%
52	9.807	2707	2711	2712	rBV3	1573	1122	0.05%	0.006%
53	9.910	2738	2743	2745	rVB5	1623	1281	0.05%	0.007%
54	10.019	2774	2777	2779	rBV3	1388	1092	0.04%	0.006%
55	10.138	2811	2814	2817	rBV3	2375	2118	0.09%	0.011%
56	10.257	2835	2851	2878	rVV	739371	1186795	47.70%	6.147%
57	10.412	2895	2899	2902	rBV6	2563	2315	0.09%	0.012%
58	10.543	2934	2940	2943	rBV7	1858	1915	0.08%	0.010%
59	10.781	3006	3014	3018	rBV9	2288	2905	0.12%	0.015%
60	10.852	3034	3036	3042	rVB7	1835	1664	0.07%	0.009%
61	10.884	3044	3046	3048	rVV2	2024	1315	0.05%	0.007%
62	10.897	3048	3050	3057	rVV6	3714	3409	0.14%	0.018%
63	10.929	3057	3060	3063	rVV3	1663	1411	0.06%	0.007%
64	10.955	3065	3068	3074	rVB7	3195	2592	0.10%	0.013%
65	11.016	3084	3087	3089	rBV4	1990	1069	0.04%	0.006%
66	11.035	3091	3093	3098	rVV5	2052	1405	0.06%	0.007%
67	11.129	3119	3122	3128	rVV6	1859	2015	0.08%	0.010%
68	11.196	3138	3143	3145	rBV4	1990	1850	0.07%	0.010%
69	11.209	3145	3147	3151	rVB4	2038	1371	0.06%	0.007%
70	11.238	3153	3156	3159	rBV3	1293	1134	0.05%	0.006%
71	11.289	3159	3172	3192	rBV	1108616	1720691	69.16%	8.912%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121719\
 Data File : VV014102.D
 Acq On : 17 Dec 2019 18:43
 Operator : SY/MD
 Sample : K6314-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.489	3231	3234	3240	rBV7	1928	1941	0.08%	0.010%
73	11.666	3277	3289	3308	rVV	1091289	1717897	69.04%	8.898%
74	11.971	3380	3384	3387	rBV5	1597	1476	0.06%	0.008%
75	12.157	3434	3442	3447	rBV10	5583	8203	0.33%	0.042%
76	12.203	3454	3456	3459	rVB3	2808	1239	0.05%	0.006%
77	12.260	3471	3474	3478	rBV3	1764	1330	0.05%	0.007%
78	12.280	3478	3480	3484	rBV5	1540	1177	0.05%	0.006%
79	12.505	3548	3550	3552	rBV3	1772	1080	0.04%	0.006%
80	12.659	3596	3598	3601	rBV4	1565	1243	0.05%	0.006%
81	12.926	3673	3681	3689	rVB5	14997	23067	0.93%	0.119%
82	13.000	3700	3704	3711	rVB9	2931	3710	0.15%	0.019%
83	13.087	3724	3731	3741	rVB9	9571	18053	0.73%	0.094%
84	13.257	3779	3784	3793	rVB9	5079	7646	0.31%	0.040%
85	13.312	3796	3801	3809	rVB9	8324	11193	0.45%	0.058%
86	13.415	3828	3833	3844	rVB9	6331	9778	0.39%	0.051%
87	13.656	3903	3908	3916	rVB7	6117	7383	0.30%	0.038%
88	13.752	3930	3938	3941	rBV7	8956	11894	0.48%	0.062%
89	13.913	3986	3988	3992	rBV5	1949	1438	0.06%	0.007%
90	14.019	4017	4021	4024	rBV5	2557	2579	0.10%	0.013%
91	14.077	4035	4039	4044	rVB7	3084	2885	0.12%	0.015%
92	14.151	4049	4062	4075	rVB10	15719	36035	1.45%	0.187%
93	14.479	4156	4164	4174	rVB7	13750	24128	0.97%	0.125%
94	14.569	4190	4192	4200	rVB8	2938	3188	0.13%	0.017%
95	14.601	4200	4202	4204	rBV3	2660	1591	0.06%	0.008%
96	14.659	4215	4220	4223	rBV6	9094	9602	0.39%	0.050%
97	14.903	4294	4296	4299	rBV3	2698	2133	0.09%	0.011%
98	15.283	4412	4414	4415	rBV2	2977	1335	0.05%	0.007%
99	15.360	4433	4438	4439	rBV4	4105	3649	0.15%	0.019%
100	15.585	4506	4508	4510	rBV3	3359	1838	0.07%	0.010%


Sum of corrected areas: 19306568

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121719\
Data File : VV014102.D
Acq On : 17 Dec 2019 18:43
Operator : SY/MD
Sample : K6314-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF13

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

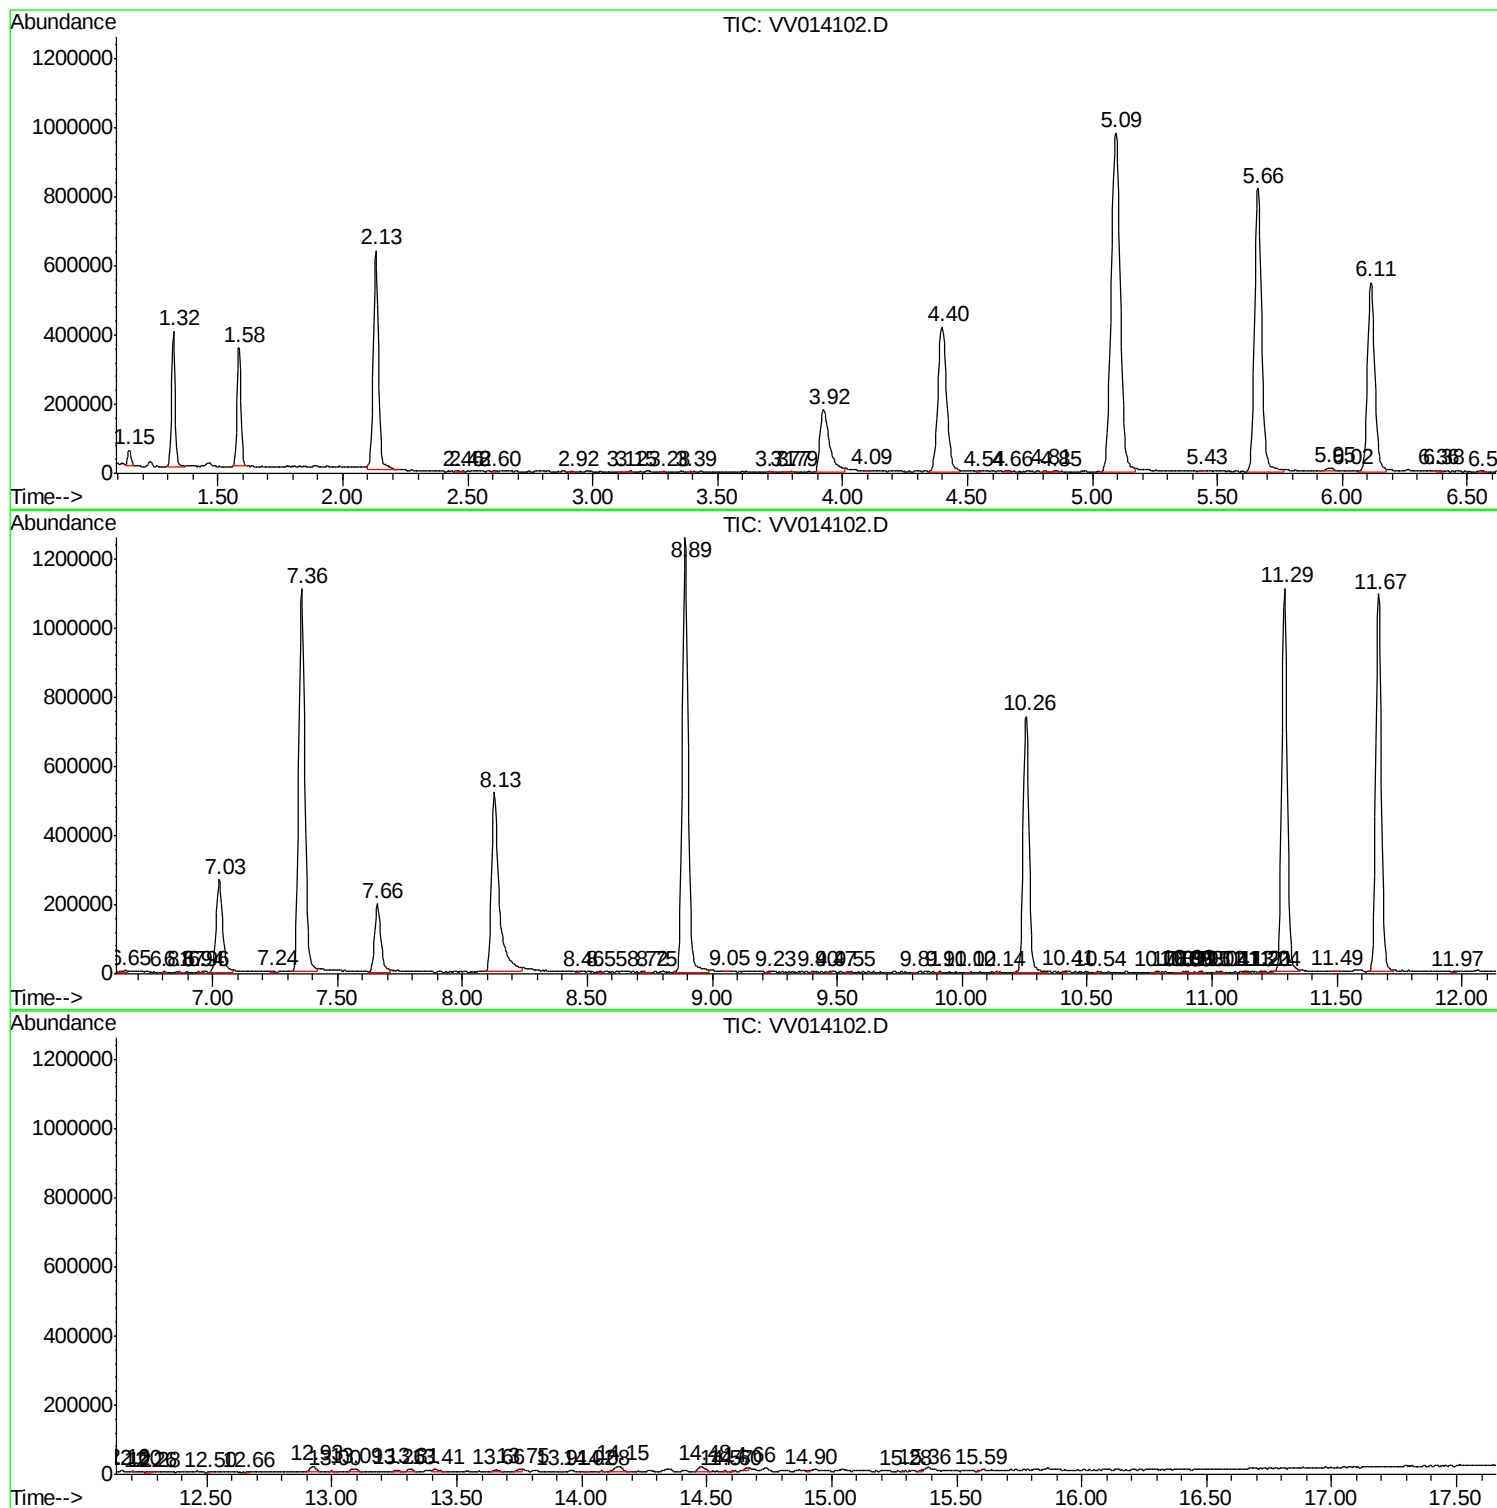

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014102.D
Acq On : 17 Dec 2019 18:43
Operator : SY/MD
Sample : K6314-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121719\
Data File : VV014102.D
Acq On : 17 Dec 2019 18:43
Operator : SY/MD
Sample : K6314-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc