


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121719\
 Data File : VV014081.D
 Acq On : 17 Dec 2019 09:25
 Operator : SY/MD
 Sample : BFB83
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 18 06:35:10 2019

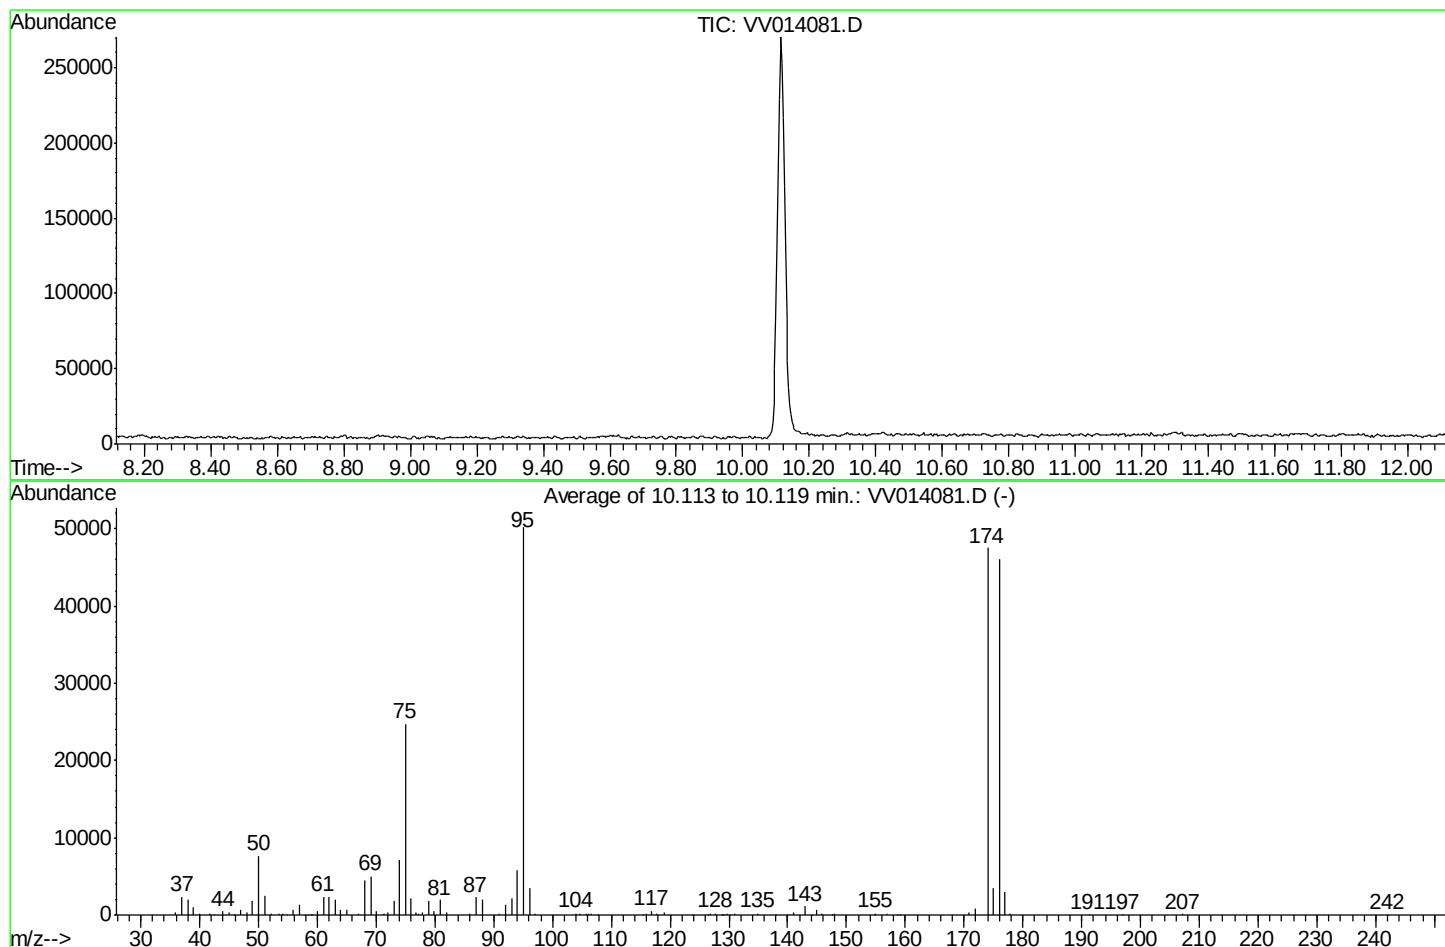

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	7670	PASS
75	95	30	80	49.3	24738	PASS
95	95	100	100	100.0	50181	PASS
96	95	5	9	7.0	3534	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.7	47514	PASS
175	174	5	9	7.3	3488	PASS
176	174	95	101	97.1	46144	PASS
177	176	5	9	6.5	3020	PASS

m/z	Abundance
35.80	641.0
37.00	2425.0
38.00	2271.0
39.00	1020.0
40.00	954.0
41.70	127.0
42.30	137.0
44.00	1037.0
45.00	426.0
45.90	265.0
47.00	746.0
48.10	350.0
49.00	2042.0
50.10	7942.0
51.00	2673.0
52.20	211.0
53.40	161.0
54.20	140.0
56.00	829.0
57.00	1446.0
58.60	103.0
58.90	102.0
60.10	496.0
61.00	2337.0
62.10	2525.0
63.00	1976.0
63.90	600.0
65.00	549.0
66.90	169.0
68.00	4423.0
69.00	5245.0
70.00	524.0
71.30	206.0
72.00	333.0
73.00	1785.0
74.00	7448.0
75.00	24728.0
76.00	2100.0
76.70	326.0
77.20	369.0
77.80	400.0
79.00	1832.0
79.90	559.0
80.90	1848.0
81.90	378.0
85.90	151.0
87.00	2318.0
88.00	2112.0
90.80	178.0
92.10	1279.0
93.00	2202.0
94.00	5689.0
95.00	50320.0
96.10	3670.0
96.90	162.0
104.00	331.0
104.80	111.0
106.10	274.0
107.70	116.0
115.90	180.0
116.80	474.0
117.80	216.0
118.90	348.0
123.80	102.0
126.30	157.0
126.80	181.0
127.80	174.0
128.70	103.0
129.10	122.0
129.70	231.0
130.10	183.0
131.00	148.0
134.90	204.0
138.00	102.0
139.80	144.0
141.10	436.0
143.00	1185.0
144.00	131.0
144.90	696.0
145.80	122.0
147.90	218.0
154.60	122.0
155.00	252.0
156.80	173.0
159.10	124.0
170.80	348.0
171.90	758.0
174.00	46864.0
174.90	3426.0
176.00	45128.0
177.00	2873.0
177.80	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

191.20	107.0
207.30	115.0
242.00	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	519.0
37.00	2449.0
38.00	2166.0
39.00	1065.0
40.00	1047.0
41.60	159.0
44.00	1141.0
45.00	462.0
45.90	241.0
47.00	735.0
48.00	353.0
49.00	1864.0
50.10	7956.0
51.00	2451.0
52.10	227.0
53.40	148.0
54.10	115.0
56.00	790.0
57.00	1335.0
60.10	495.0
61.00	2421.0
62.00	2426.0
63.00	2068.0
63.90	666.0
64.90	702.0
67.00	159.0
68.00	4609.0
69.00	5149.0
70.00	531.0
71.30	183.0
72.10	345.0
73.00	1938.0
74.10	7291.0
75.00	25824.0
76.00	2128.0
76.80	335.0
77.20	432.0
77.90	339.0
78.90	1951.0
79.90	565.0
80.90	1985.0
81.90	407.0
85.90	196.0
87.00	2409.0
88.00	2254.0
90.90	219.0
92.00	1447.0
93.00	2355.0
94.00	6020.0
95.00	52048.0
96.10	3743.0
97.00	193.0
104.00	230.0
104.70	120.0
105.80	225.0
106.70	139.0
115.80	154.0
116.90	535.0
117.80	255.0
119.00	403.0
126.70	228.0
127.80	223.0
129.70	217.0
130.90	126.0
134.90	212.0
139.80	112.0
141.00	405.0
143.00	1144.0
144.00	124.0
144.90	649.0
145.80	133.0
148.00	169.0
155.00	187.0
156.80	204.0
158.70	110.0
170.80	312.0
171.90	915.0
174.00	49056.0
174.90	3571.0
176.00	47640.0
177.00	3114.0
177.80	204.0
197.00	105.0
207.20	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	509.0
37.00	2238.0
38.00	1777.0
39.00	977.0
39.90	985.0
41.70	162.0
44.00	1190.0
44.90	477.0
46.00	219.0
46.90	699.0
48.10	301.0
49.00	1567.0
50.00	7113.0
51.10	2132.0
52.10	238.0
53.40	107.0
54.20	120.0
54.90	150.0
56.00	710.0
57.00	1123.0
57.90	115.0
59.20	116.0
60.10	474.0
61.00	2432.0
62.00	2210.0
63.00	1870.0
64.00	691.0
64.90	671.0
67.10	157.0
68.00	4272.0
69.10	4643.0
70.00	435.0
71.20	144.0
72.10	373.0
73.00	1886.0
74.10	6579.0
75.00	23664.0
76.00	2028.0
76.90	306.0
77.20	319.0
77.90	283.0
78.90	1862.0
79.90	531.0
80.90	1958.0
81.90	385.0
85.90	190.0
87.00	2188.0
88.00	1852.0
90.90	267.0
92.00	1420.0
93.00	2170.0
94.00	5827.0
95.00	48176.0
96.10	3191.0
97.10	269.0
104.00	158.0
104.60	126.0
105.80	183.0
106.70	187.0
115.40	112.0
115.90	102.0
116.90	495.0
117.80	220.0
119.00	438.0
126.70	155.0
127.80	231.0
129.80	168.0
134.90	147.0
141.00	366.0
143.00	1053.0
145.00	569.0
145.90	130.0
147.60	108.0
148.10	123.0
154.80	162.0
156.90	192.0
158.70	139.0
170.90	320.0
172.00	1003.0
174.00	46624.0
174.90	3467.0
176.00	45664.0
177.00	3073.0
177.90	219.0
207.10	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.20	163.0
35.90	201.0
37.50	108.0
38.40	159.0
39.10	101.0
40.00	875.0
44.10	698.0
45.10	104.0
45.90	200.0
48.70	121.0
51.30	119.0
54.40	104.0
55.90	108.0
62.70	103.0
75.40	100.0
77.40	149.0
83.10	115.0
108.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83