




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024061.D
 Acq On : 17 Dec 2021 13:53
 Operator : SY/MD
 Sample : M5113-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLV6

Manual IntegrationsAPPROVED

Quant Time: Dec 18 01:45:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

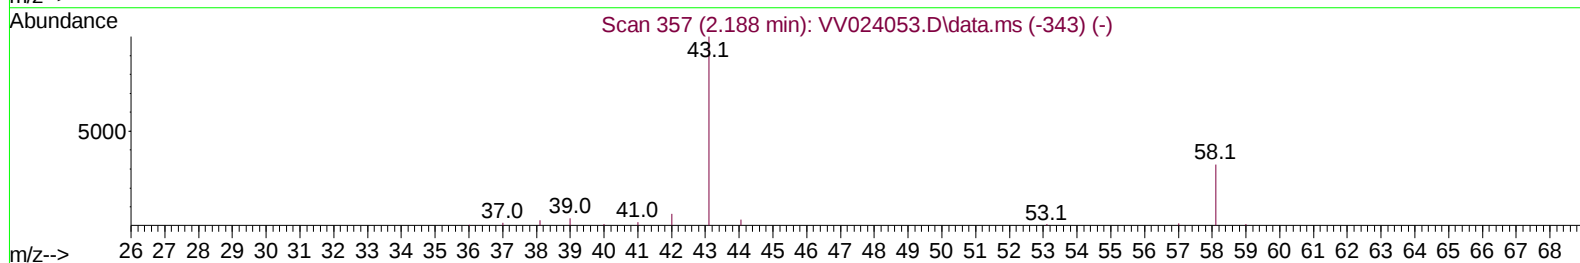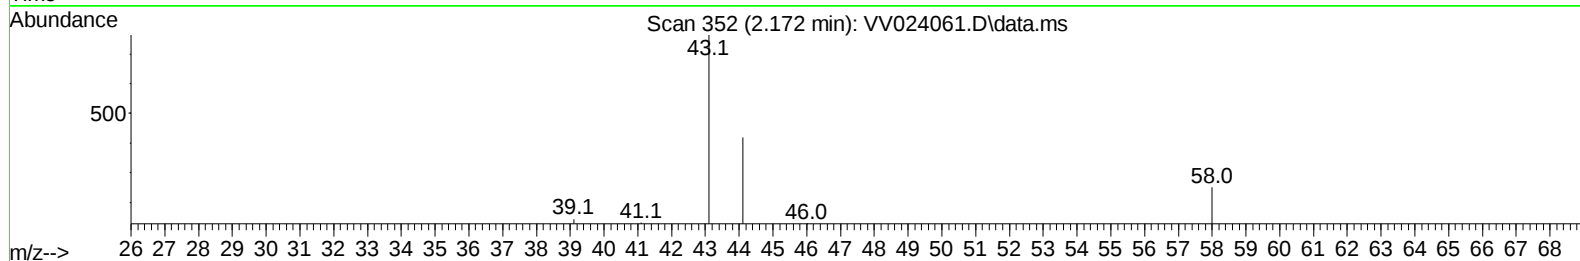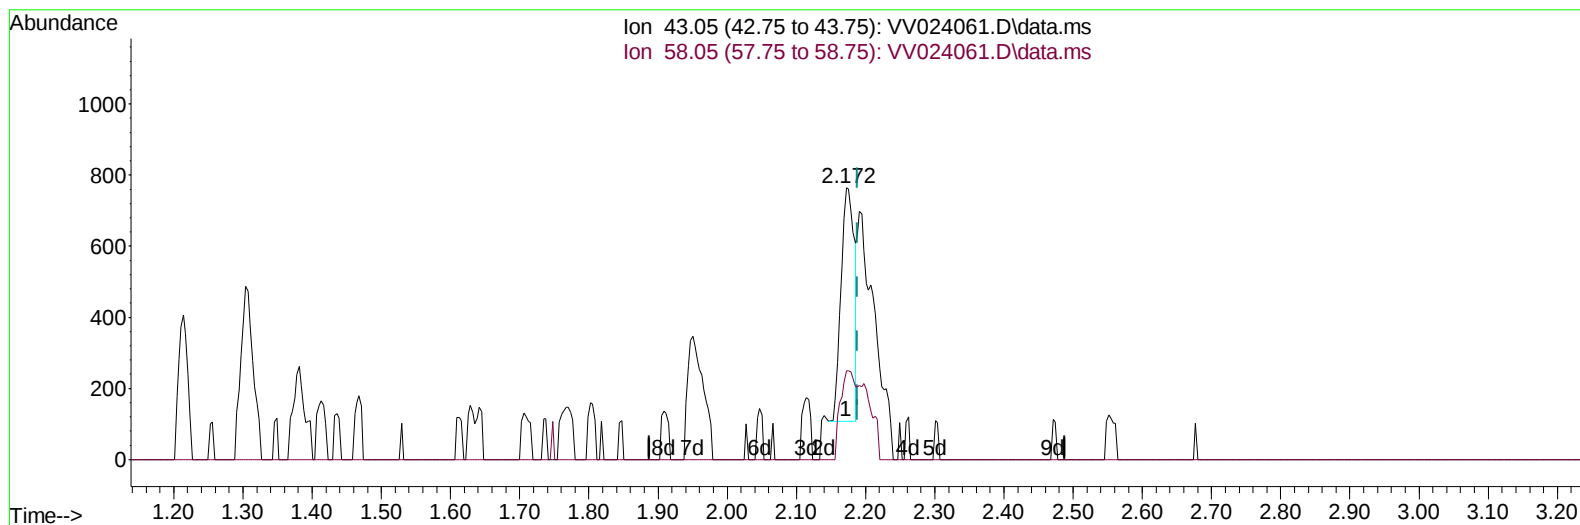

TIC: VV024061.D\data.ms

(13) Acetone (T)

2.172min (-0.016) 1.12 ug/L

response 860

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	46.16#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024061.D
 Acq On : 17 Dec 2021 13:53
 Operator : SY/MD
 Sample : M5113-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLV6

Manual IntegrationsAPPROVED

Quant Time: Dec 18 01:45:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

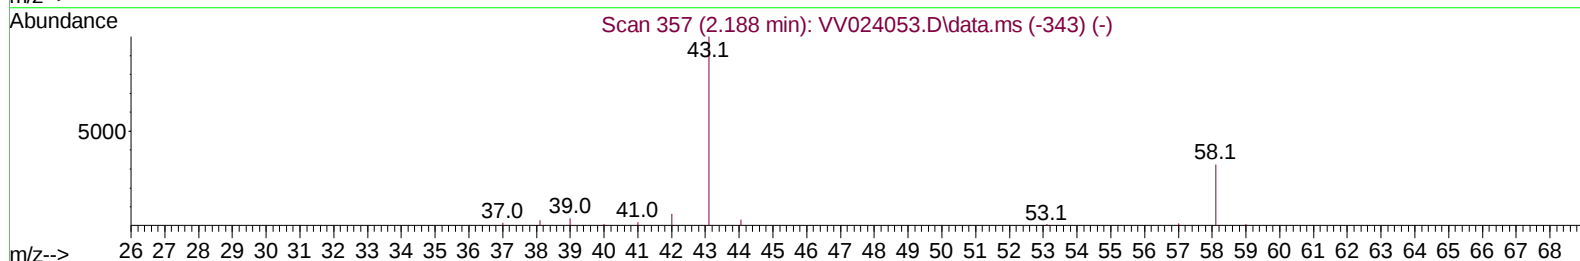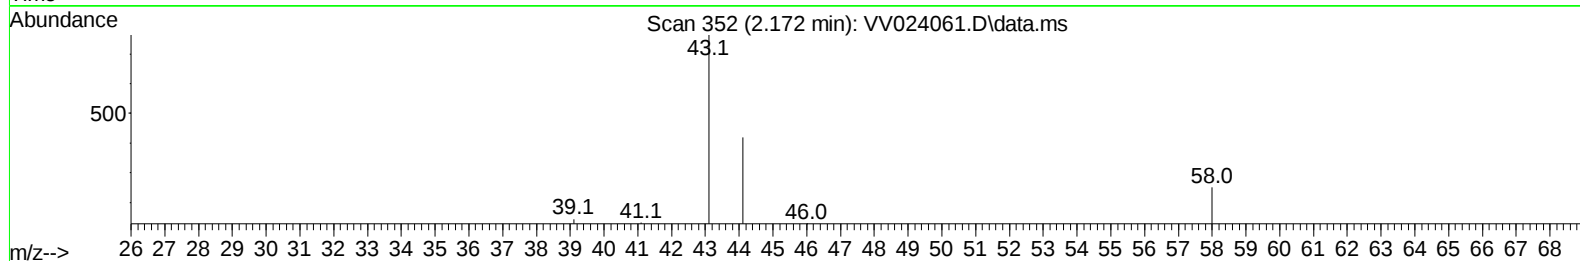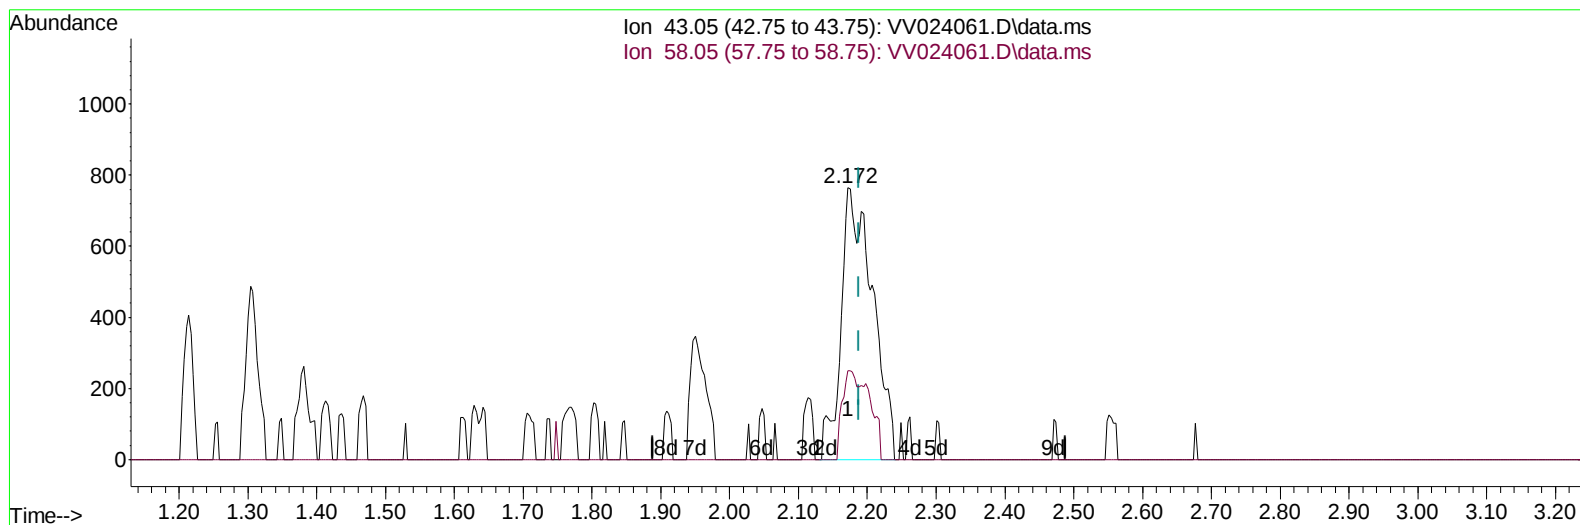

TIC: VV024061.D\data.ms

(13) Acetone (T)

2.172min (-0.016) 3.16 ug/L m

response 2435

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	16.30
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024061.D
 Acq On : 17 Dec 2021 13:53
 Operator : SY/MD
 Sample : M5113-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLV6

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 12/22/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Quant Time: Dec 18 01:45:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	91613	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	93333	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46409	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	21824	4.431	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	88.600%	
7) Chloroethane-d5	1.568	69	19483	4.741	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.108	63	33199	3.453	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	69.000%	
20) 2-Butanone-d5	3.895	46	44708	46.464	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	92.920%	
24) Chloroform-d	4.349	84	51231	4.592	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	5.037	65	25040	4.821	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.400%	
32) Benzene-d6	5.050	84	95290	5.155	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.000%	
36) 1,2-Dichloropropane-d6	6.069	67	27731	4.972	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	99.400%	
41) Toluene-d8	7.317	98	83914	5.042	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	100.800%	
43) trans-1,3-Dichloroprop...	7.625	79	9623	4.159	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.088	63	34327	33.142	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	66.280%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18287	3.953	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	79.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	32427	5.231	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	104.600%	
Target Compounds						
13) Acetone	2.172	43	2435m	3.163	ug/L	
33) Benzene	5.104	78	9075	0.344	ug/L	100
51) Chlorobenzene	8.882	112	11011	0.554	ug/L	93
60) Isopropylbenzene	9.934	105	2937	0.108	ug/L #	97
63) 1,2,4-Trimethylbenzene	10.918	105	2212	0.098	ug/L	100
65) 1,4-Dichlorobenzene	11.271	146	2152	0.154	ug/L	92
67) 1,2-Dichlorobenzene	11.641	146	1791	0.140	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024061.D
Acq On : 17 Dec 2021 13:53
Operator : SY/MD
Sample : M5113-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLV6

Manual IntegrationsAPPROVED

Quant Time: Dec 18 01:45:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 18 01:42:59 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

