




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024073.D
 Acq On : 17 Dec 2021 18:40
 Operator : SY/MD
 Sample : M5133-05DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH5DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 18 01:48:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

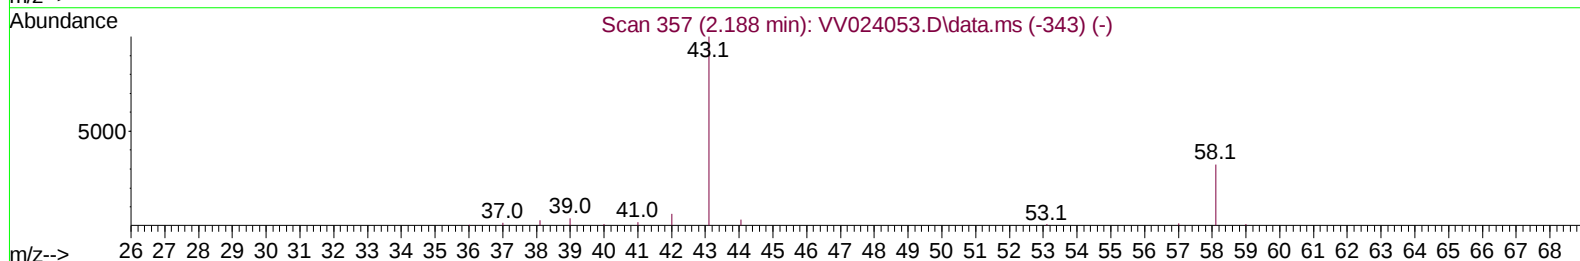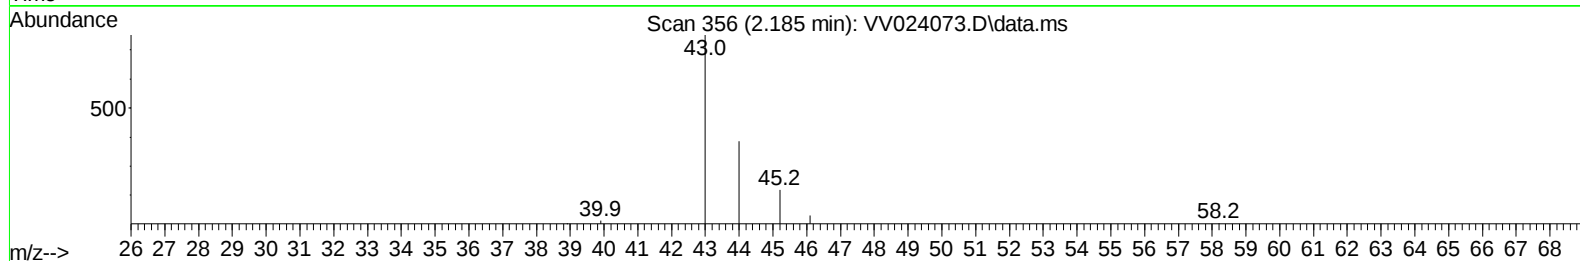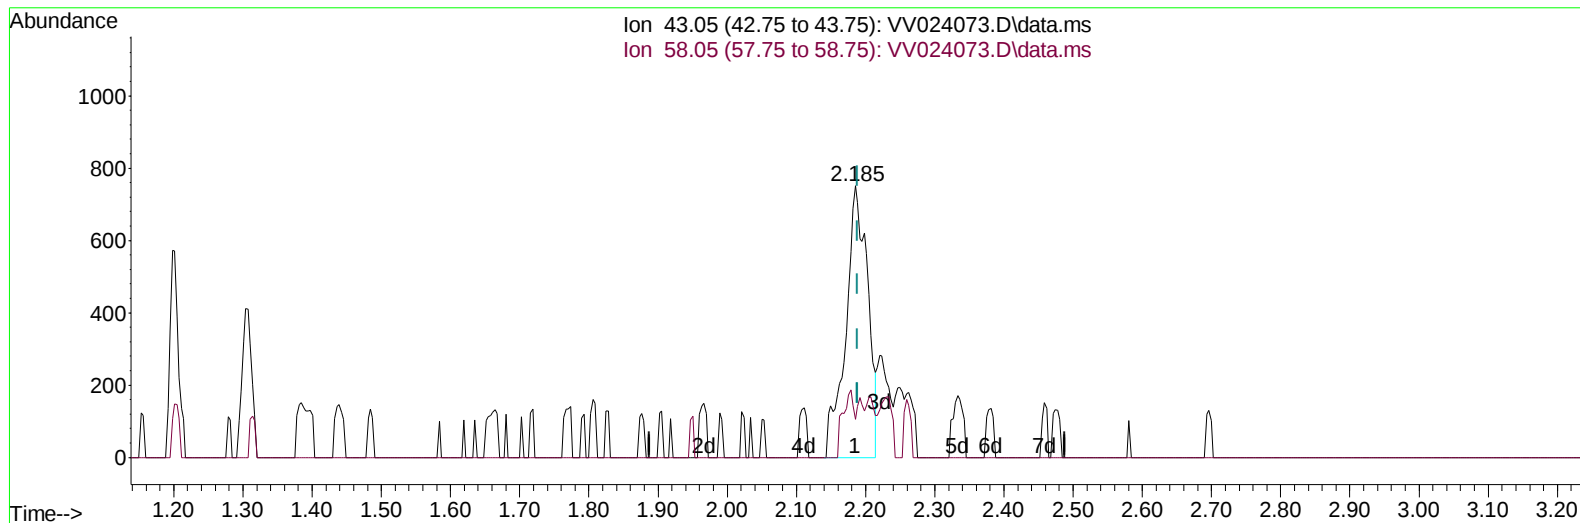

TIC: VV024073.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 2.32 ug/L

response 1654

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	6.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024073.D
 Acq On : 17 Dec 2021 18:40
 Operator : SY/MD
 Sample : M5133-05DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH5DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 18 01:48:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

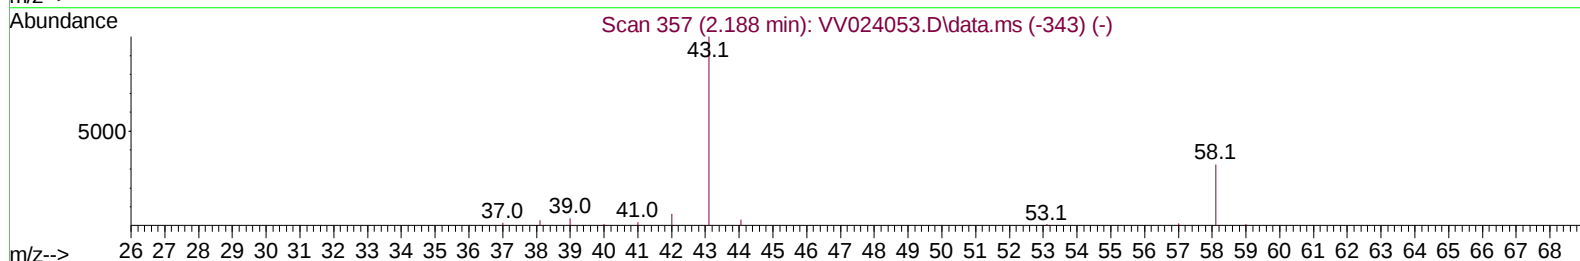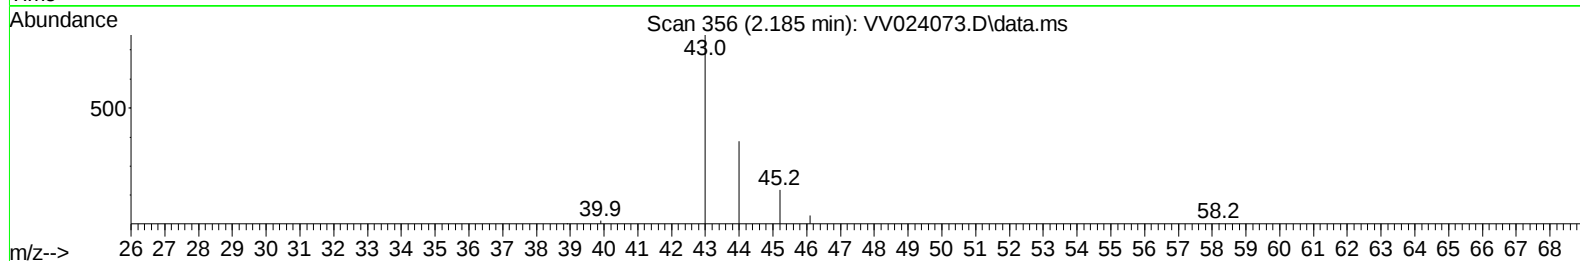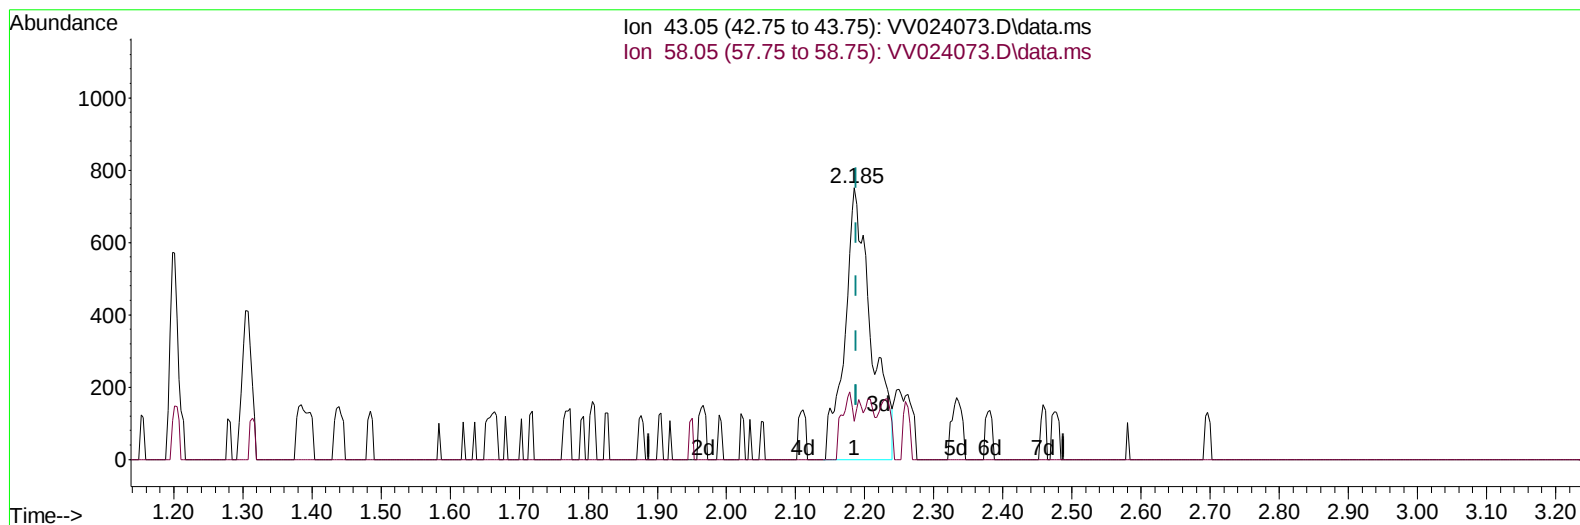

TIC: VV024073.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 2.79 ug/L m

response	1994	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	5.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024073.D
 Acq On : 17 Dec 2021 18:40
 Operator : SY/MD
 Sample : M5133-05DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH5DL

Manual IntegrationsAPPROVED

Quant Time: Dec 18 01:48:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	84923	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	91652	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	45801	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	20113	4.406	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	88.200%		
7) Chloroethane-d5	1.568	69	18190	4.775	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	95.600%		
11) 1,1-Dichloroethene-d2	2.105	63	32136	3.606	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	72.200%		
20) 2-Butanone-d5	3.902	46	36064	40.433	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	80.860%		
24) Chloroform-d	4.349	84	49582	4.795	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.800%		
26) 1,2-Dichloroethane-d4	5.034	65	25378	5.271	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	105.400%		
32) Benzene-d6	5.050	84	87857	4.840	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.800%		
36) 1,2-Dichloropropane-d6	6.069	67	26665	4.869	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.400%		
41) Toluene-d8	7.317	98	77811	4.761	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	95.200%		
43) trans-1,3-Dichloroprop...	7.625	79	10416	4.584	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	91.600%		
46) 2-Hexanone-d5	8.088	63	37230	36.604	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	73.200%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18459	4.063	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	81.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	31215	5.102	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	102.000%		
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	1994m	2.794	ug/L	
16) Methylene chloride	2.507	84	2909	0.390	ug/L	84
31) Carbon tetrachloride	4.828	117	79250	7.031	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024073.D
Acq On : 17 Dec 2021 18:40
Operator : SY/MD
Sample : M5133-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBH5DL

Manual IntegrationsAPPROVED

Quant Time: Dec 18 01:48:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 18 01:42:59 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

