

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121721\
 Data File : VW024068.D
 Acq On : 17 Dec 2021 16:40
 Operator : SY/MD
 Sample : M5133-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBH6

Quant Time: Dec 18 01:47:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	83624	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	89442	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	44149	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	19312	4.296	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.000%
7) Chloroethane-d5	1.565	69	18244	4.864	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.105	63	32549	3.709	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.200%
20) 2-Butanone-d5	3.896	46	47470	54.048	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.100%
24) Chloroform-d	4.349	84	48805	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.034	65	25714	5.424	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.400%
32) Benzene-d6	5.050	84	89746	5.066	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
36) 1,2-Dichloropropane-d6	6.069	67	26472	4.953	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.317	98	78330	4.911	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
43) trans-1,3-Dichloroprop...	7.625	79	9720	4.384	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.600%
46) 2-Hexanone-d5	8.088	63	38231	38.516	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.040%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18403	4.151	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	31678	5.372	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds						Qvalue
13) Acetone	2.182	43	9831	13.991	ug/L	87
31) Carbon tetrachloride	4.828	117	86231	7.839	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024068.D
Acq On : 17 Dec 2021 16:40
Operator : SY/MD
Sample : M5133-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBH6

Quant Time: Dec 18 01:47:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 18 01:42:59 2021
Response via : Initial Calibration

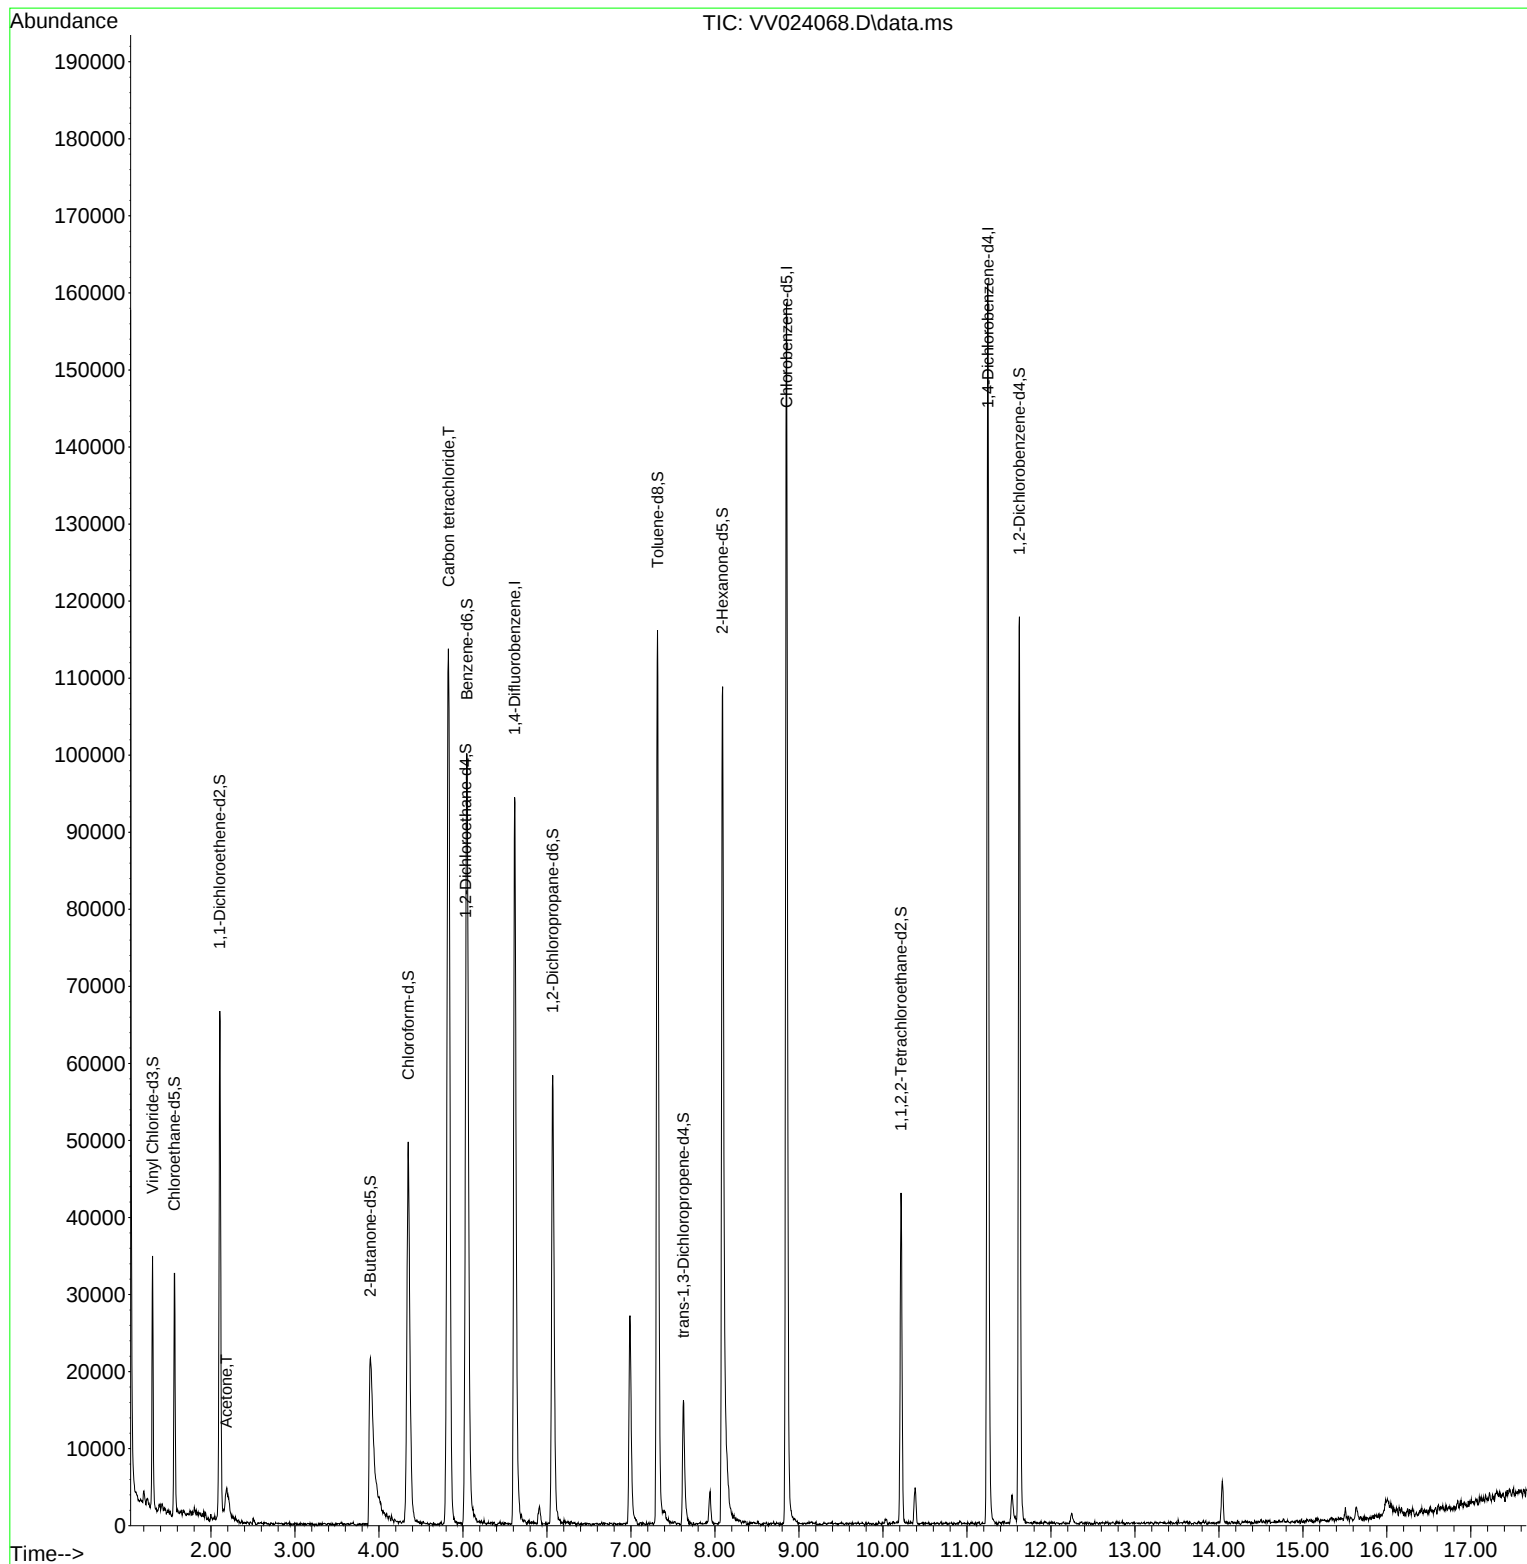

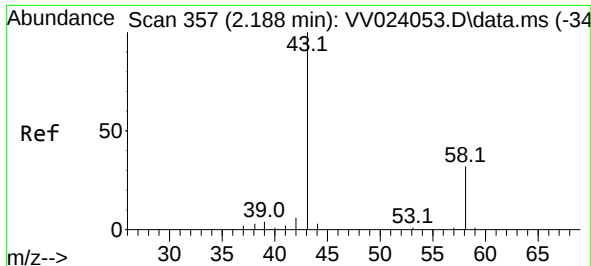

#13

Acetone

Concen: 13.991 ug/L

RT: 2.182 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV024068.D

Acq: 17 Dec 2021 16:40

Instrument :

MSVOA_V

ClientSampleId :





GBBH6

Tgt Ion: 43 Resp: 9831

Ion Ratio Lower Upper

43 100

58 26.8 0.0 41.4

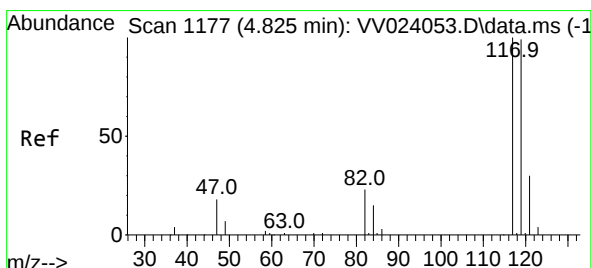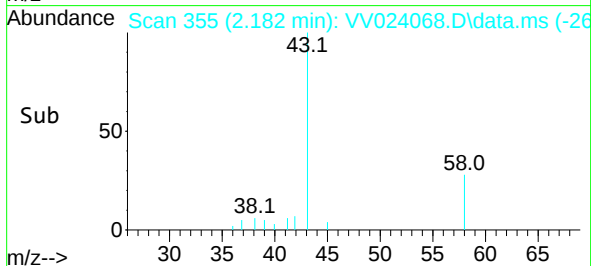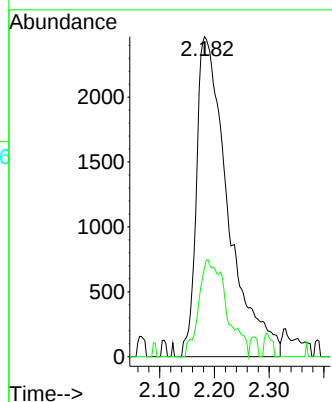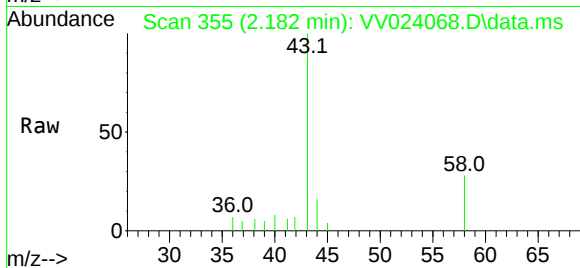

#31

Carbon tetrachloride

Concen: 7.839 ug/L

RT: 4.828 min Scan# 1178

Delta R.T. 0.003 min

Lab File: VV024068.D

Acq: 17 Dec 2021 16:40

Tgt Ion: 117 Resp: 86231

Ion Ratio Lower Upper

117 100

119 97.7 76.6 114.8

