

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121721\
 Data File : VW024071.D
 Acq On : 17 Dec 2021 17:52
 Operator : SY/MD
 Sample : M5133-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBBJ2

Quant Time: Dec 18 01:47:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 18 01:42:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	86745	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	92353	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	45726	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	20554	4.408	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.200%
7) Chloroethane-d5	1.568	69	18100	4.652	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.108	63	32554	3.576	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.899	46	48770	53.530	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.060%
24) Chloroform-d	4.352	84	47909	4.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
26) 1,2-Dichloroethane-d4	5.034	65	24704	5.023	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.053	84	89354	4.885	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	6.072	67	27068	4.905	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%
41) Toluene-d8	7.317	98	77757	4.722	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.625	79	9862	4.308	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.088	63	38085	37.160	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.320%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	19592	4.280	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	32107	5.257	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
13) Acetone	2.188	43	9984	13.697	ug/L	80
31) Carbon tetrachloride	4.828	117	167733	14.768	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024071.D
Acq On : 17 Dec 2021 17:52
Operator : SY/MD
Sample : M5133-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBBJ2

Quant Time: Dec 18 01:47:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 18 01:42:59 2021
Response via : Initial Calibration




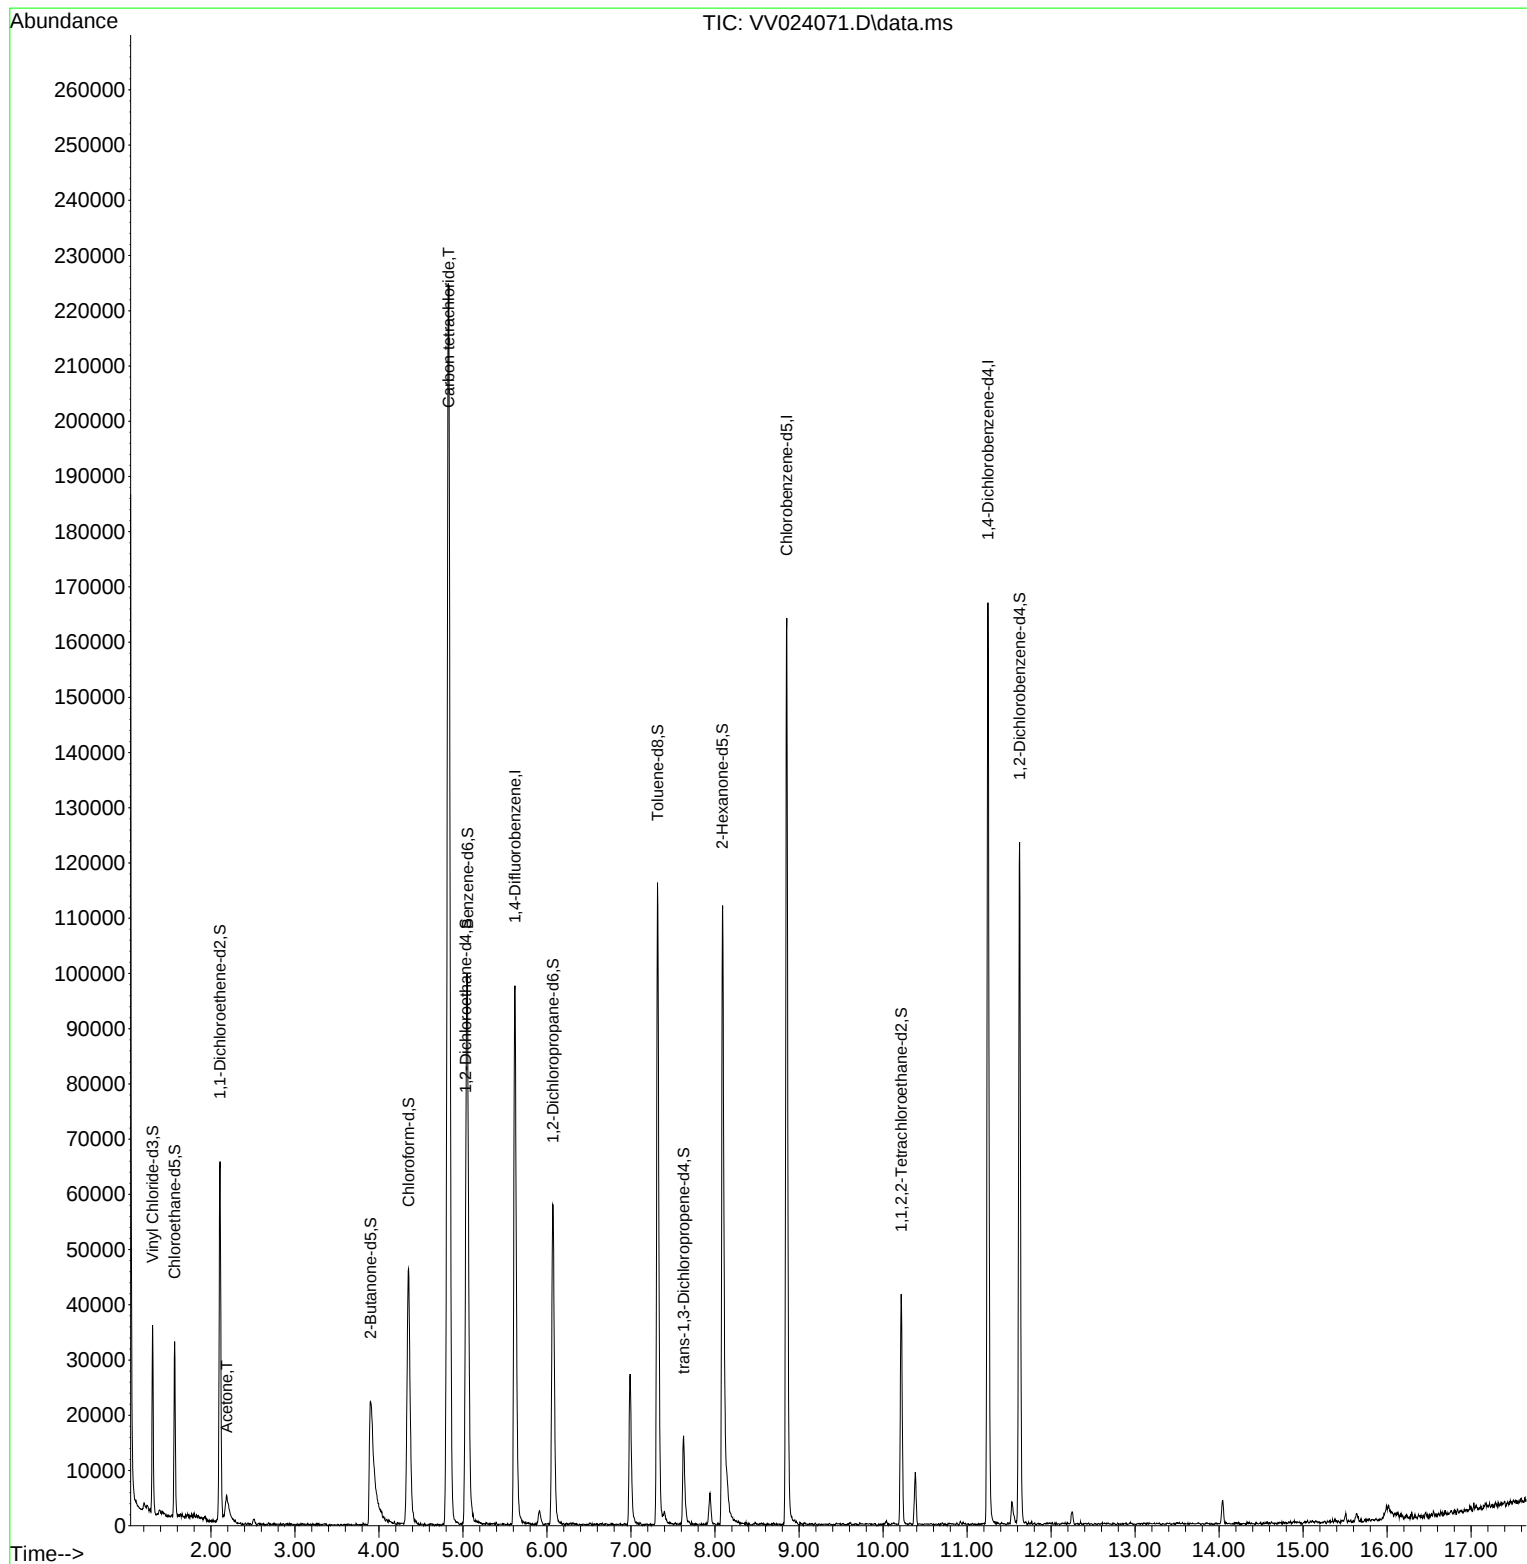


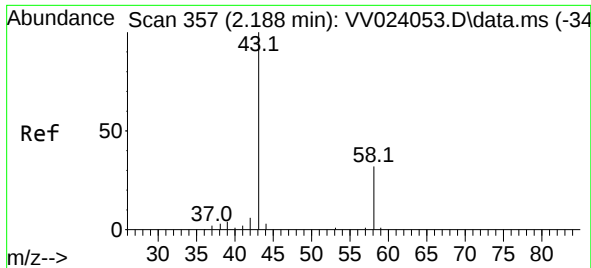

#13
Acetone
Concen: 13.697 ug/L
RT: 2.188 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV024071.D
Acq: 17 Dec 2021 17:52

Instrument :
MSVOA_V
ClientSampleId :
GBBJ2

Tgt Ion: 43 Resp: 9984
Ion Ratio Lower Upper
43 100
58 11.5 0.0 41.4

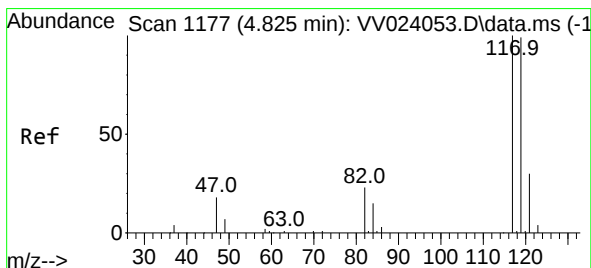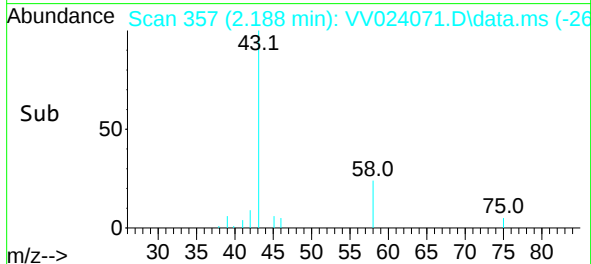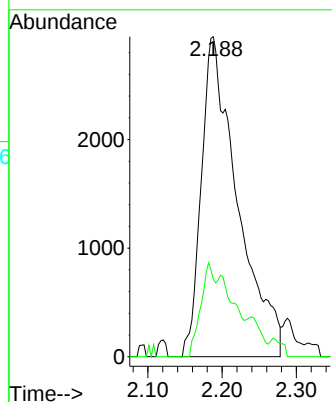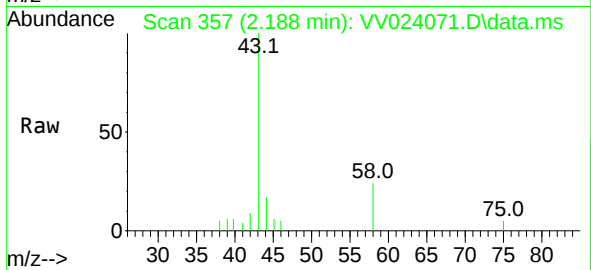

#31
Carbon tetrachloride
Concen: 14.768 ug/L
RT: 4.828 min Scan# 1178
Delta R.T. 0.003 min
Lab File: VV024071.D
Acq: 17 Dec 2021 17:52

Tgt Ion: 117 Resp: 167733
Ion Ratio Lower Upper
117 100
119 96.0 76.6 114.8

