

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024056.D
 Acq On : 17 Dec 2021 11:55
 Operator : SY/MD
 Sample : M5090-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3E1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	94	rBV	40722	39604	14.64%	1.693%
2	1.381	101	106	116	rBV5	2087	3553	1.31%	0.152%
3	1.564	156	163	178	rVB	33538	37987	14.04%	1.624%
4	2.105	321	331	346	rBV	68347	99404	36.75%	4.249%
5	2.182	346	355	369	rVB2	3674	8876	3.28%	0.379%
6	3.899	877	889	912	rBV3	23654	83288	30.79%	3.560%
7	4.346	1012	1028	1057	rBV	52901	134254	49.63%	5.739%
8	5.047	1230	1246	1275	rBV3	103745	265353	98.09%	11.343%
9	5.616	1412	1423	1448	rBV	101299	203293	75.15%	8.690%
10	5.905	1504	1513	1525	rBV7	2965	5937	2.19%	0.254%
11	6.069	1552	1564	1589	rBV2	59235	123642	45.71%	5.286%
12	6.989	1840	1850	1871	rBV2	28450	53560	19.80%	2.290%
13	7.317	1940	1952	1970	rBV	123104	216335	79.97%	9.248%
14	7.397	1970	1977	1988	rVB2	5233	9211	3.40%	0.394%
15	7.625	2039	2048	2065	rBV3	16086	29277	10.82%	1.252%
16	7.937	2136	2145	2160	rVB2	3370	5889	2.18%	0.252%
17	8.091	2183	2193	2227	rBV	95674	196689	72.71%	8.408%
18	8.850	2418	2429	2454	rBV	163431	270521	100.00%	11.564%
19	9.551	2637	2647	2657	rBV8	1896	2950	1.09%	0.126%
20	10.217	2842	2854	2866	rBV2	37606	60119	22.22%	2.570%
21	10.381	2892	2905	2916	rBV4	7427	11866	4.39%	0.507%
22	10.918	3064	3072	3082	rVB3	2972	4012	1.48%	0.172%
23	11.249	3163	3175	3195	rBV	169454	263166	97.28%	11.250%
24	11.535	3256	3264	3269	rBV7	3169	4449	1.64%	0.190%
25	11.625	3281	3292	3310	rBV	120447	190206	70.31%	8.131%
26	14.040	4034	4043	4054	rVB2	3061	5102	1.89%	0.218%
27	15.506	4491	4499	4509	rVB5	4647	7364	2.72%	0.315%
28	15.982	4638	4647	4650	rBV6	1896	3358	1.24%	0.144%




Sum of corrected areas: 2339265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024056.D
Acq On : 17 Dec 2021 11:55
Operator : SY/MD
Sample : M5090-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

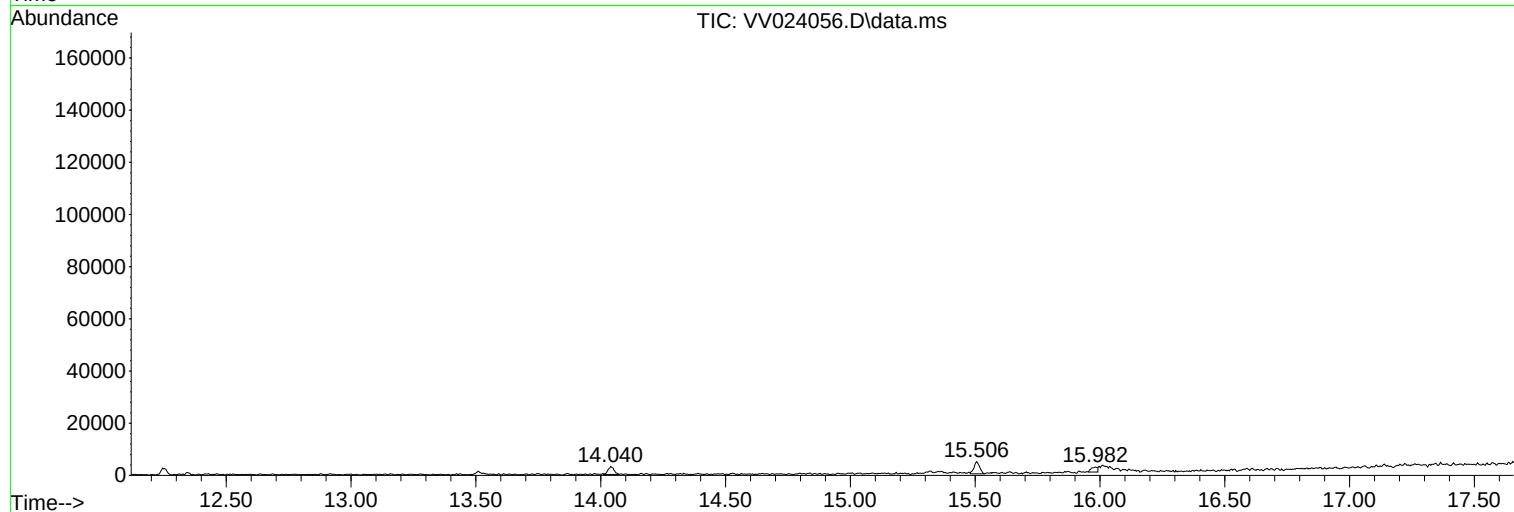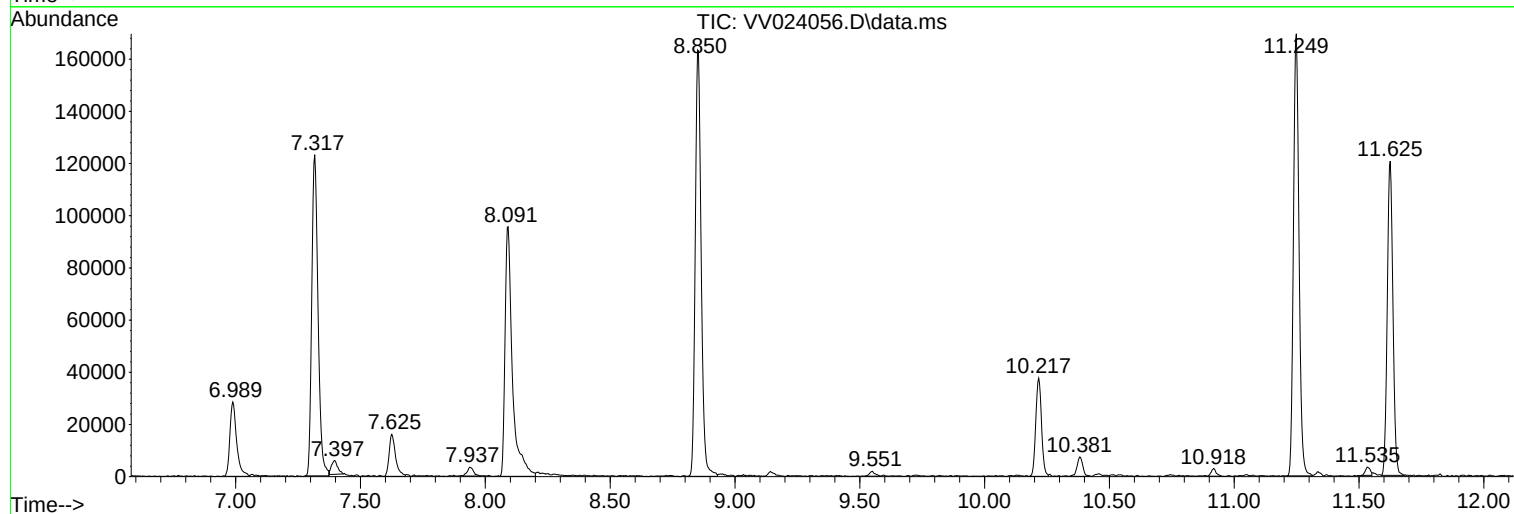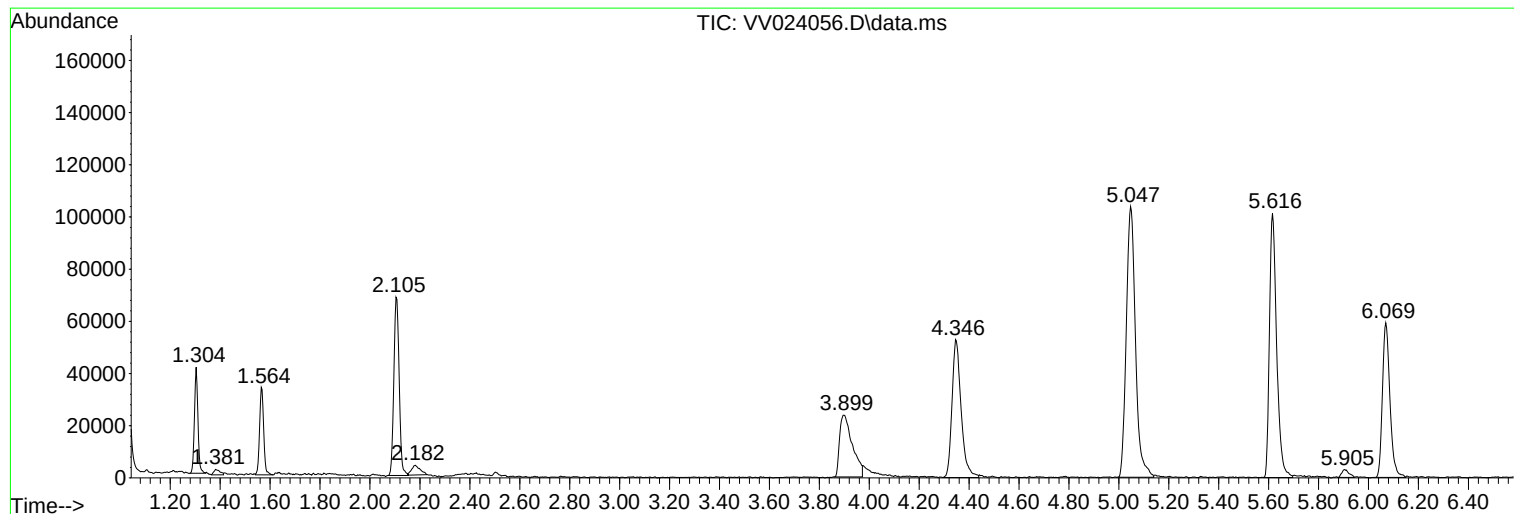

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024056.D
Acq On : 17 Dec 2021 11:55
Operator : SY/MD
Sample : M5090-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024056.D
Acq On : 17 Dec 2021 11:55
Operator : SY/MD
Sample : M5090-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc