

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024061.D
 Acq On : 17 Dec 2021 13:53
 Operator : SY/MD
 Sample : M5113-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLV6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	38245	39477	12.78%	1.641%
2	1.568	156	164	174	rBV	31782	37050	11.99%	1.540%
3	1.953	276	284	291	rVB3	4145	5863	1.90%	0.244%
4	2.108	321	332	342	rBV	67559	97433	31.53%	4.049%
5	3.895	872	888	915	rBV2	26717	89707	29.03%	3.728%
6	4.352	1014	1030	1051	rBV	51244	122266	39.57%	5.081%
7	5.050	1230	1247	1290	rBV3	105703	283857	91.87%	11.797%
8	5.616	1411	1423	1445	rBV2	100808	207966	67.31%	8.643%
9	5.911	1504	1515	1517	rBV4	2749	3724	1.21%	0.155%
10	6.069	1549	1564	1581	rBV2	61033	125434	40.60%	5.213%
11	6.989	1839	1850	1868	rBV2	28384	53006	17.16%	2.203%
12	7.317	1941	1952	1969	rBV	125461	215935	69.89%	8.974%
13	7.400	1970	1978	1984	rVB6	2265	3686	1.19%	0.153%
14	7.625	2038	2048	2068	rBV2	16050	31545	10.21%	1.311%
15	8.091	2183	2193	2224	rBV	104052	203980	66.02%	8.477%
16	8.853	2418	2430	2460	rBV	169031	308968	100.00%	12.840%
17	9.934	2758	2766	2777	rVB2	4408	6413	2.08%	0.267%
18	10.217	2843	2854	2868	rBV	39858	63579	20.58%	2.642%
19	10.384	2891	2906	2913	rBV7	2334	4303	1.39%	0.179%
20	10.918	3064	3072	3080	rVB3	3070	4728	1.53%	0.196%
21	11.095	3118	3127	3135	rBV5	2276	3459	1.12%	0.144%
22	11.188	3147	3156	3165	rBV4	2904	4576	1.48%	0.190%
23	11.249	3165	3175	3192	rVV	169387	270970	87.70%	11.261%
24	11.455	3231	3239	3245	rBV3	3118	4378	1.42%	0.182%
25	11.625	3277	3292	3311	rBV	125680	200189	64.79%	8.320%
26	12.879	3675	3682	3691	rVB4	5858	8005	2.59%	0.333%
27	15.506	4492	4499	4508	rVB5	3716	5716	1.85%	0.238%




Sum of corrected areas: 2406213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024061.D
Acq On : 17 Dec 2021 13:53
Operator : SY/MD
Sample : M5113-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLV6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

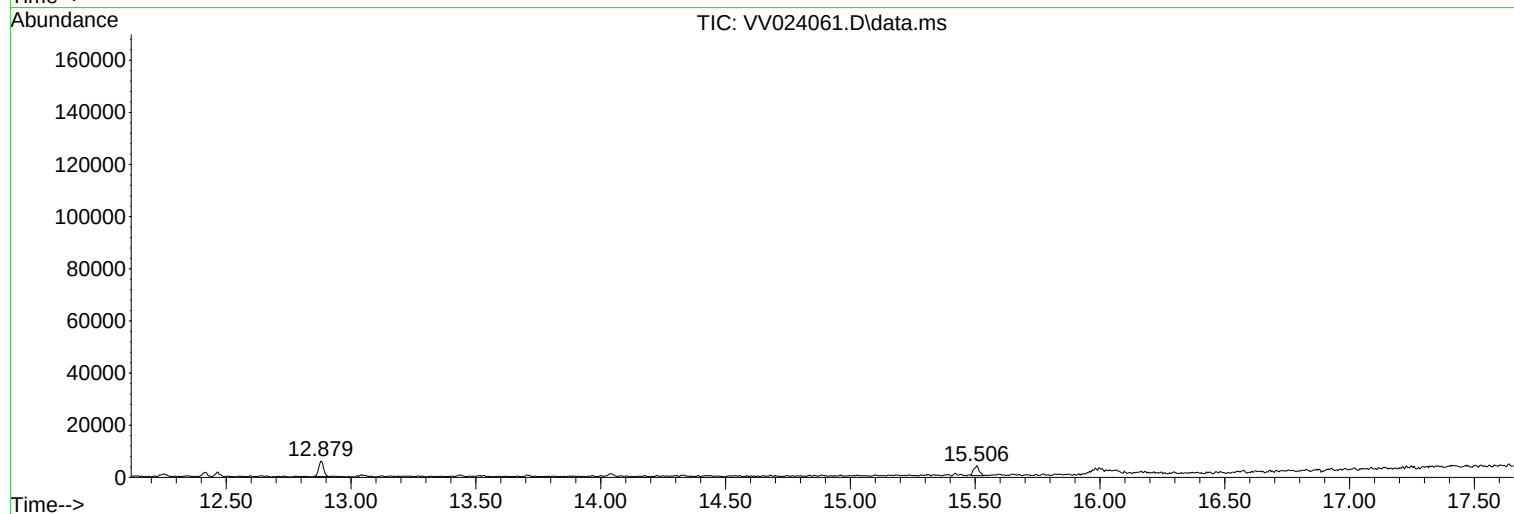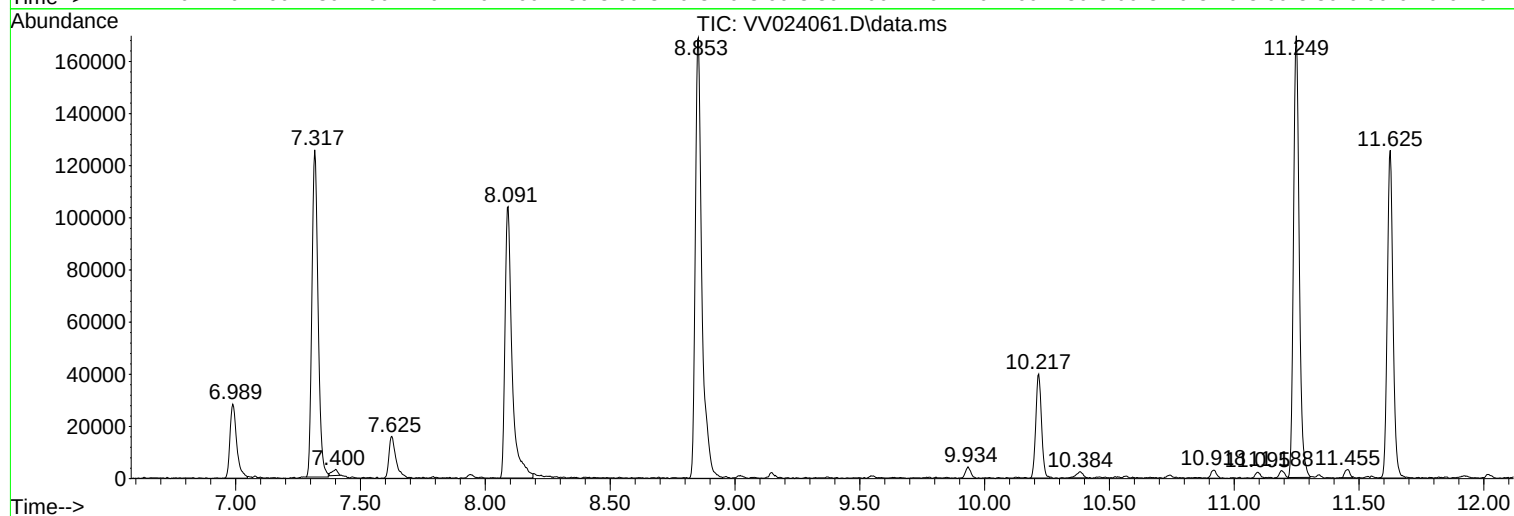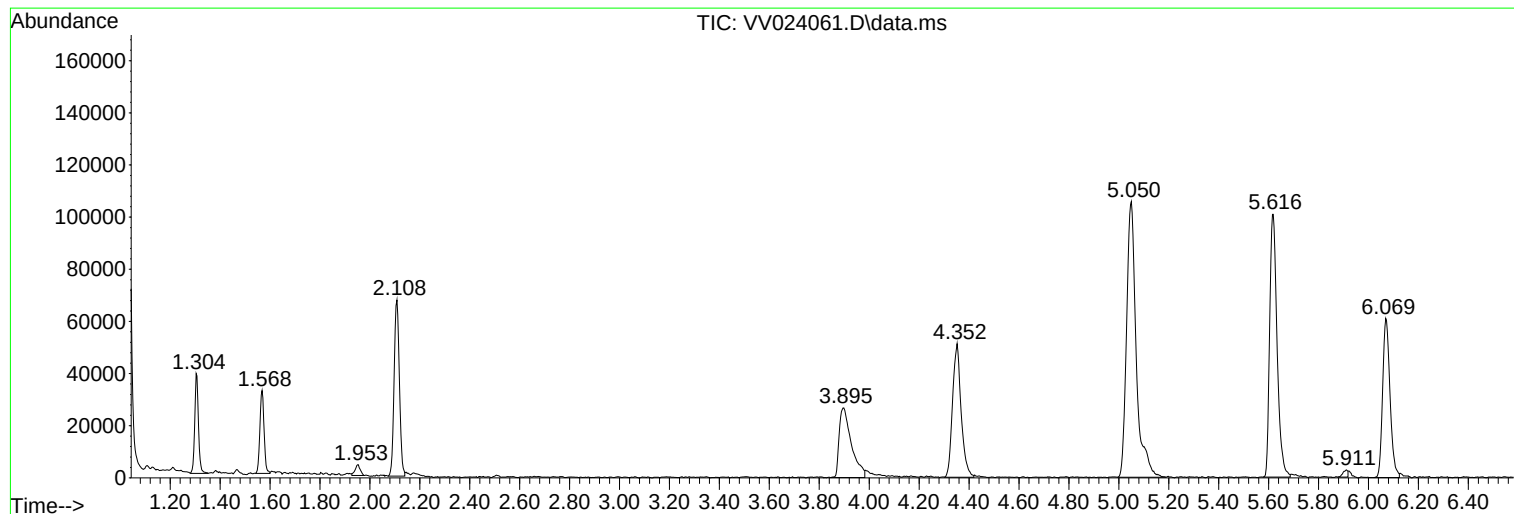

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024061.D
Acq On : 17 Dec 2021 13:53
Operator : SY/MD
Sample : M5113-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLV6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024061.D
Acq On : 17 Dec 2021 13:53
Operator : SY/MD
Sample : M5113-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLV6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc