

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
 Data File : VV024062.D
 Acq On : 17 Dec 2021 14:17
 Operator : SY/MD
 Sample : M5090-15DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3C7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	29	rVB	10268	8919	1.66%	0.314%
2	1.214	49	54	62	rVB	6142	5895	1.10%	0.208%
3	1.307	73	83	97	rVB2	61813	67526	12.60%	2.381%
4	1.568	156	164	175	rBV	33134	38044	7.10%	1.341%
5	2.108	320	332	348	rBV	69065	100952	18.84%	3.560%
6	2.507	447	456	469	rBV2	10857	17630	3.29%	0.622%
7	2.761	524	535	553	rBV3	16695	31293	5.84%	1.103%
8	3.908	878	892	922	rBV2	209328	535851	100.00%	18.895%
9	4.352	1013	1030	1053	rVB2	50063	124844	23.30%	4.402%
10	5.047	1230	1246	1276	rBV2	104753	264728	49.40%	9.335%
11	5.616	1411	1423	1449	rBV	103857	209643	39.12%	7.392%
12	6.069	1551	1564	1583	rBV2	59975	124192	23.18%	4.379%
13	6.989	1838	1850	1865	rBV2	28254	52538	9.80%	1.853%
14	7.317	1939	1952	1969	rBV	125311	219927	41.04%	7.755%
15	7.625	2039	2048	2070	rBV2	15795	29430	5.49%	1.038%
16	8.092	2181	2193	2231	rBV	84023	204615	38.19%	7.215%
17	8.854	2417	2430	2451	rBV	162707	276546	51.61%	9.751%
18	10.217	2841	2854	2867	rBV2	39404	62477	11.66%	2.203%
19	11.249	3164	3175	3193	rBV	171405	265878	49.62%	9.375%
20	11.625	3281	3292	3309	rBV	120817	195018	36.39%	6.877%




Sum of corrected areas: 2835946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024062.D
Acq On : 17 Dec 2021 14:17
Operator : SY/MD
Sample : M5090-15DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

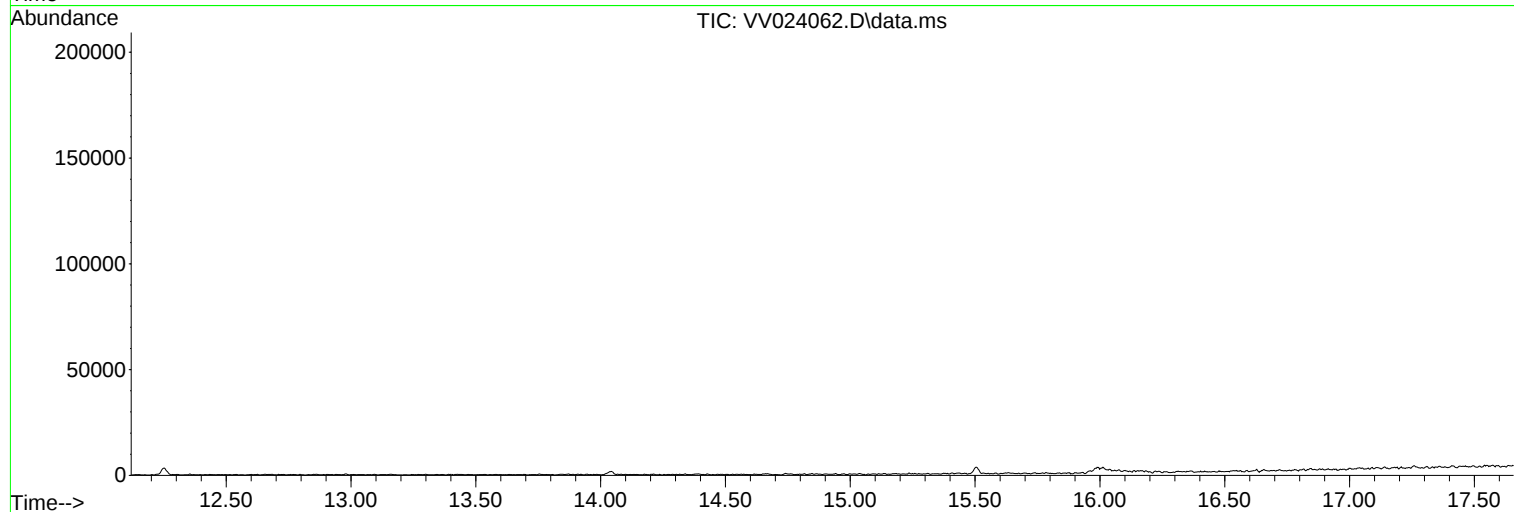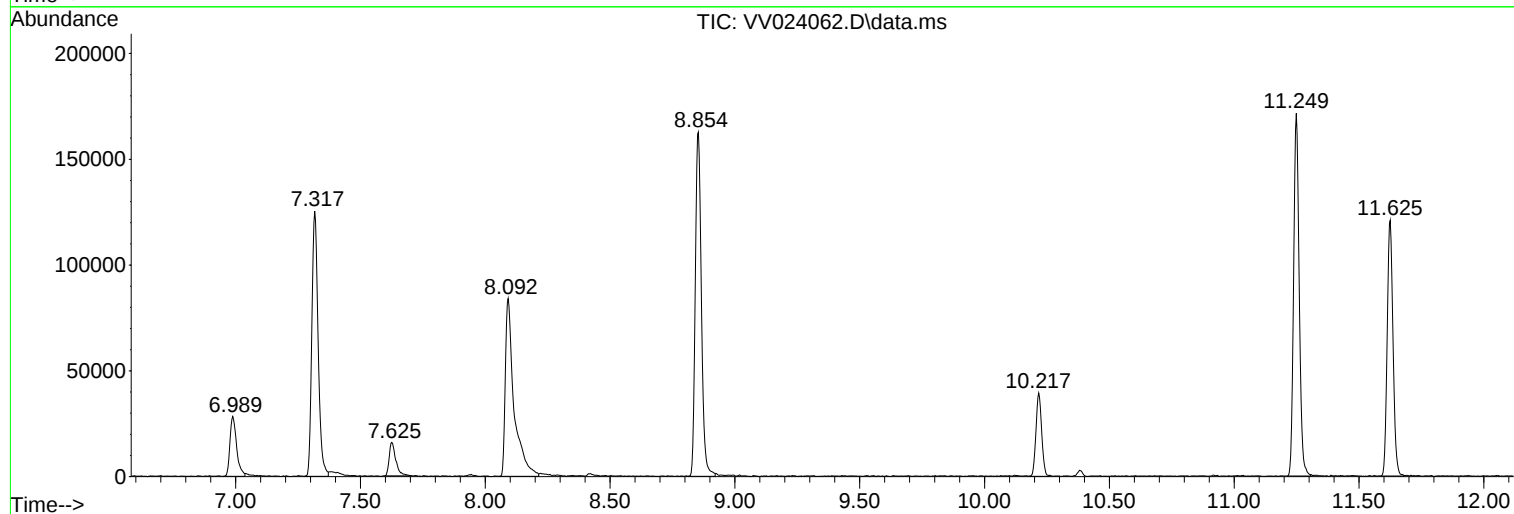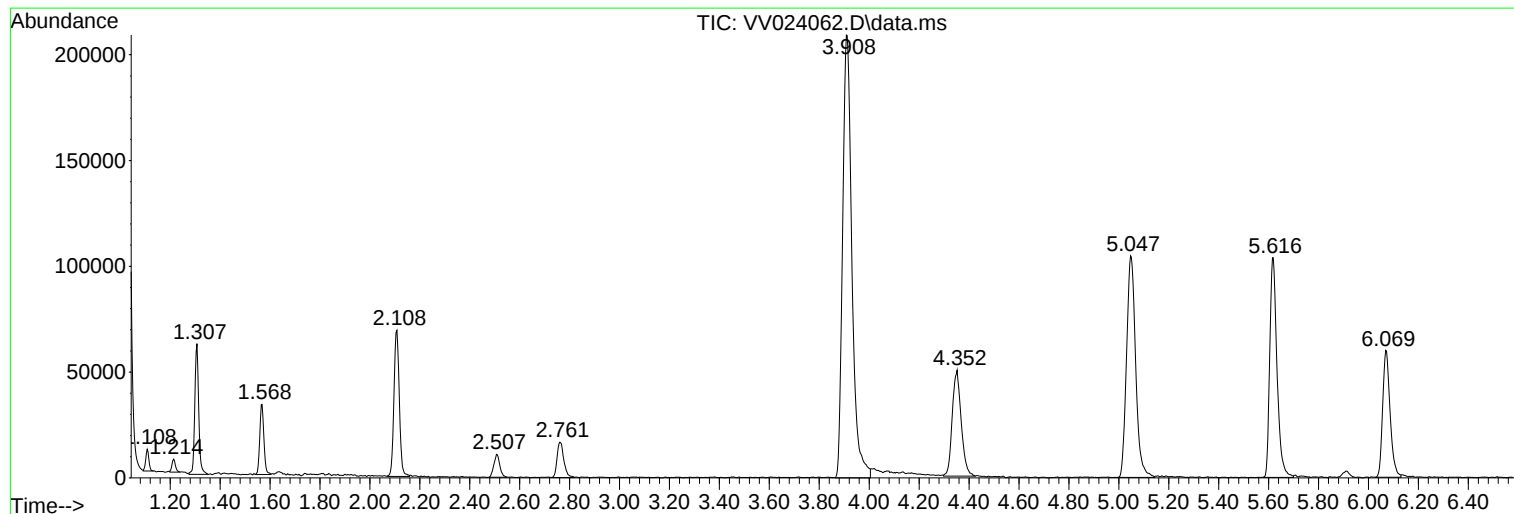

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024062.D
Acq On : 17 Dec 2021 14:17
Operator : SY/MD
Sample : M5090-15DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121721\
Data File : VV024062.D
Acq On : 17 Dec 2021 14:17
Operator : SY/MD
Sample : M5090-15DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc